

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

NI-9242

CALIBRATION PROCEDURE

NI 9242/9244

4-Channel, 250 V_{rms}/400 V_{rms} L-N or 800 V_{rms} L-L, 24-Bit,
Simultaneous Analog Input Module

Français	Deutsch	日本語	한국어	简体中文
ni.com/manuals				

This document contains the verification and adjustment procedures for the National Instruments 9242 and National Instruments 9244. In this document, the NI 9242 and NI 9244 are inclusively referred to as NI 9242/9244. For more information about calibration solutions, visit ni.com/calibration.

Contents

Software.....	1
Documentation.....	2
Test Equipment.....	3
Test Conditions.....	3
Initial Setup.....	4
Verification.....	4
Accuracy Verification.....	4
Adjustment.....	6
Accuracy Adjustment.....	7
EEPROM Update.....	8
Reverification.....	8
Accuracy Under Calibration Conditions.....	8
Worldwide Support and Services.....	9

Software

Calibrating the NI 9242/9244 requires the installation of NI-DAQmx 9.9 or later on the calibration system. You can download NI-DAQmx from ni.com/downloads. NI-DAQmx supports LabVIEW, LabWindows™/CVI™, ANSI C, and .NET. When you install NI-DAQmx, you only need to install support for the application software that you intend to use.

Documentation

Consult the following documents for information about the NI 9242/9244, NI-DAQmx, and your application software. All documents are available on ni.com and help files install with the software.



NI cDAQ-9174/9178 Quick Start Guide
NI-DAQmx installation and hardware setup



NI 9242 User Manual and Specifications
NI 9242 specific information, specifications, and calibration interval



NI 9244 User Manual and Specifications
NI 9244 specific information, specifications, and calibration interval



NI-DAQmx Readme
Operating system and application software support in NI-DAQmx



LabVIEW Help
LabVIEW programming concepts and reference information about NI-DAQmx VIs and functions



NI-DAQmx C Reference Help
Reference information for NI-DAQmx C functions and NI-DAQmx C properties



NI-DAQmx .NET Help Support for Visual Studio
Reference information for NI-DAQmx .NET methods and NI-DAQmx .NET properties, key concepts, and a C enum to .NET enum mapping table

Test Equipment

Table 1 lists the equipment recommended for the performance verification and adjustment procedures. If the recommended equipment is not available, select a substitute using the requirements listed in Table 1.

Table 1. Recommended Equipment

Equipment	Recommended Model	Requirements
Calibrator	Fluke 5500A	Use a high-precision voltage source with an accuracy ≤ 57 ppm and offset error < 2 mV.
Connector Backshell	NI 9967	Use the NI 9967 to ensure circuits connected to the NI 9242 are properly insulated from human contact.
	NI 9969	Use the NI 9969 to ensure circuits connected to the NI 9244 are properly insulated from human contact.
Chassis	NI cDAQ-9178	—

Test Conditions

The following setup and environmental conditions are required to ensure the NI 9242/9244 meets published specifications.

- Keep connections to the NI 9242/9244 as short as possible. Long cables and wires act as antennas, picking up extra noise that can affect measurements.
- Verify that all connections to the 9242/9244 are secure.
- Use shielded copper wire for all cable connections to the NI 9242/9244. Use twisted-pairs wire to eliminate noise and thermal offsets.
- Maintain an ambient temperature of $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$. The NI 9242/9244 temperature will be greater than the ambient temperature.
- Keep relative humidity below 80%.
- Allow a warm-up time of at least 10 minutes to ensure that the NI 9242/9244 measurement circuitry is at a stable operating temperature.

Initial Setup

Complete the following steps to set up the NI 9242/9244.

1. Install NI-DAQmx.
2. Make sure the NI cDAQ-9178 power source is not connected.
3. Connect the NI cDAQ-9178 to the system safety ground.
 - a. Attach a ring lug to a 14 AWG (1.6 mm) wire.
 - b. Connect the ring lug to the ground terminal on the side of the NI cDAQ-9178 using the ground screw.
 - c. Attach the other end of the wire to the system safety ground.
4. Install the module in slot 8 of the NI cDAQ-9178 chassis. Leave slots 1 through 7 of the NI cDAQ-9178 chassis empty.
5. Connect the NI cDAQ-9178 chassis to your host computer.
6. Connect the power source to the NI cDAQ-9178 chassis.
7. Launch Measurement & Automation Explorer (MAX).
8. Right-click the device name and select **Self-Test** to ensure that the module is working properly.

Verification

The following performance verification procedure describes the sequence of operation and test points required to verify the NI 9242/9244 and assumes that adequate traceable uncertainties are available for the calibration references.




Caution Verification requires that hazardous voltages be connected to the NI 9242/9244. Refer to the *NI 9242 User Manual and Specifications* or *NI 9244 User Manual and Specifications* for safety guidelines.

Accuracy Verification

Complete the following procedure to determine the As-Found status of the NI 9242/9244.

1. Set the calibrator to Standby mode (STBY).
2. Connect the NI 9242/9244 to the calibrator as shown in Figure 1. Ensure that the chassis ground lug and the calibrator LO are connected to the same ground.

Figure 1. NI 9242/9244 Calibration Connections

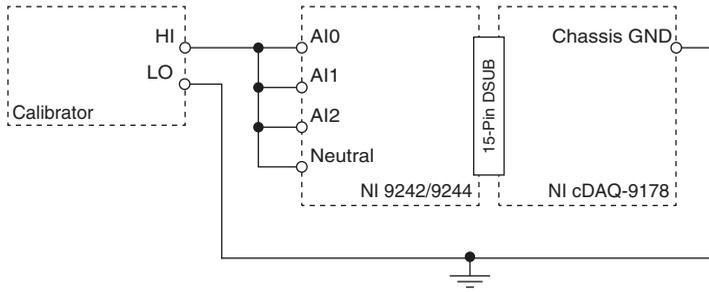

Note The chassis ground lug connection to ground is the NI 9242/9244 ground connection.

3. Set the calibrator voltage to a Test Point value indicated in Table 4 or Table 5.
4. Set the calibrator to Operate mode (OPR).
5. Acquire and average samples.
 - a. Create and configure an AI voltage task according to Table 2.

Table 2. NI 9242/9244 AI Voltage Task Configuration

Module	Minimum (V)	Maximum (V)	Physical Channels	Terminal Configuration
NI 9242	-500	500	AI0:2	NRSE
			Neutral	RSE
NI 9244	-997.5	997.5	AI0:2	NRSE
			Neutral	RSE



Note The terminal configuration of NRSE for channels AI0:2 and RSE for Neutral is the default configuration for the NI 9242/9244.

- b. Configure the task timing according to Table 3.

Table 3. NI 9242/9244 Voltage Task Timing Configuration

Sample Mode	Samples Per Channel	Rate (kS/s)
Finite Samples	5000	50

- c. Start the task.
- d. Read samples from the NI 9242/9244.
- e. Average the samples per AI channel and Neutral.

f. Perform the following calculation using the average for each AI channel.

$$AIx_{Measurement} = AIx_{Average} + Neutral_{Average}$$

g. Clear the task.

6. Compare the $Neutral_{Average}$ and the $AIx_{Measurement}$ for each AI channel to the limits in Table 4 or Table 5.
7. Set the calibrator to Standby mode (STBY).
8. Repeat steps 3 through 7 for each test point in Table 4 or Table 5.
9. Disconnect the calibrator from the device.

Table 4. NI 9242 Verification Test Limits

Test Point		1-Year Limits	
Location	Value (V)	Lower Limit (V _{DC})	Upper Limit (V _{DC})
Min	-450	-450.5447	-449.4553
Mid	0	-0.0825	0.0828
Max	450	449.4553	450.5447

Table 5. NI 9244 Verification Test Limits

Test Point		1-Year Limits	
Location	Value (V)	Lower Limit (V _{DC})	Upper Limit (V _{DC})
Min	-950	-950.9026	-949.0974
Mid	0	-0.0571	0.0571
Max	950	949.0974	950.9026



Note The test limits listed in Table 4 and Table 5 are derived using the values in Table 8.

Adjustment

The following performance adjustment procedure describes the sequence of operation required to adjust the NI 9242/9244.



Caution Adjustment requires that hazardous voltages be connected to the NI 9242/9244. Refer to the *NI 9242 User Manual and Specifications* or *NI 9244 User Manual and Specifications* for safety guidelines.

Accuracy Adjustment

Complete the following procedure to adjust the accuracy performance of the NI 9242/9244.

1. Set the calibrator to Standby mode (STBY).
2. Connect the NI 9242/9244 to the calibrator as shown in Figure 1.
3. Adjust the NI 9242/9244.
 - a. Initialize a calibration session on the NI 9242/9244. The default password is NI.
 - b. Input the external temperature in degrees Celsius.
 - c. Call the NI 9242/9244 get C Series adjustment points function to obtain an array of recommended calibration voltages for the NI 9242/9244.
 - d. Set the calibrator to a reference value determined by the array of recommended calibration voltages.
 - e. Set the calibrator to Operate mode (OPR).
 - f. Call and configure the NI 9242/9244 setup function according to Table 6.

Table 6. Setup Configuration

Physical Channel	Adjustment Point
cDAQMod8/AI0:2, cDAQMod8/Neutral	The recommended calibration voltage



Note The NI 9242/9244 acquisition starts each time the setup function is called.

- g. Call and configure the NI 9242/9244 adjustment function according to Table 7.

Table 7. Adjustment Configuration

Physical Channel	Reference Value
cDAQMod8/AI0:2, cDAQMod8/Neutral	The actual value of the voltage output of the calibrator

- h. Set the calibrator to Standby mode (STBY).
 - i. Repeat steps d through g for each point in the array.
 - j. Close the calibration session.
4. Disconnect the NI 9242/9244 from the calibrator.

EEPROM Update

When an adjustment procedure is completed, the NI 9242/9244 internal calibration memory (EEPROM) is immediately updated.

If you do not want to perform an adjustment, you can update the calibration date and onboard calibration temperature without making any adjustments by initializing an external calibration, setting the C Series calibration temperature, and closing the external calibration.

Reverification

Repeat the *Verification* section to determine the As-Left status of the device.



Note If any test fails Reverification after performing an adjustment, verify that you have met the *Test Conditions* before returning your device to NI. Refer to *Worldwide Support and Services* for assistance in returning the device to NI.

Accuracy Under Calibration Conditions

The values in the following table are based on calibrated scaling coefficients, which are stored in the onboard EEPROM.

The following accuracy table is valid for calibration under the following conditions:

- Ambient temperature $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$
- NI 9242/9244 installed in slot 8 of an NI cDAQ-9178 chassis
- Slots 1 through 7 of the NI cDAQ-9178 chassis are empty

Table 8. NI 9242/9244 Accuracy Under Calibration Conditions

Module	Percent of Reading (Gain Error)	Percent of Range* (Offset Error)
NI 9242	$\pm 0.103\%$	$\pm 0.023\%$
NI 9244	$\pm 0.089\%$	$\pm 0.01\%$

* Range equals 354 V for the NI 9242 and 565.7 V for the NI 9244.



Note For operational specifications, refer to the most recent *NI 9242 User Manual and Specifications* or *NI 9244 User Manual and Specifications* online at ni.com/manuals.

Worldwide Support and Services

The National Instruments website is your complete resource for technical support. At ni.com/support you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit ni.com/services for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit ni.com/register to register your National Instruments product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

A Declaration of Conformity (DoC) is our claim of compliance with the Council of the European Communities using the manufacturer's declaration of conformity. This system affords the user protection for electromagnetic compatibility (EMC) and product safety. You can obtain the DoC for your product by visiting ni.com/certification. If your product supports calibration, you can obtain the calibration certificate for your product at ni.com/calibration.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world. For telephone support in the United States, create your service request at ni.com/support or dial 1 866 ASK MYNI (275 6964). For telephone support outside the United States, visit the Worldwide Offices section of ni.com/niglobal to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.

Refer to the *NI Trademarks and Logo Guidelines* at ni.com/trademarks for more information on National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at ni.com/patents. You can find information about end-user license agreements (EULAs) and third-party legal notices in the readme file for your NI product. Refer to the *Export Compliance Information* at ni.com/legal/export-compliance for the National Instruments global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2014 National Instruments. All rights reserved.