

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

PXI-1052

INSTALLATION GUIDE

NI PXI-1052 Optional Rear Rack Mount Kit



Note Use this kit in conjunction with the NI PXI-1052 front rack mount kit.

To mount the NI PXI-1052 in an instrument rack, complete the following steps:

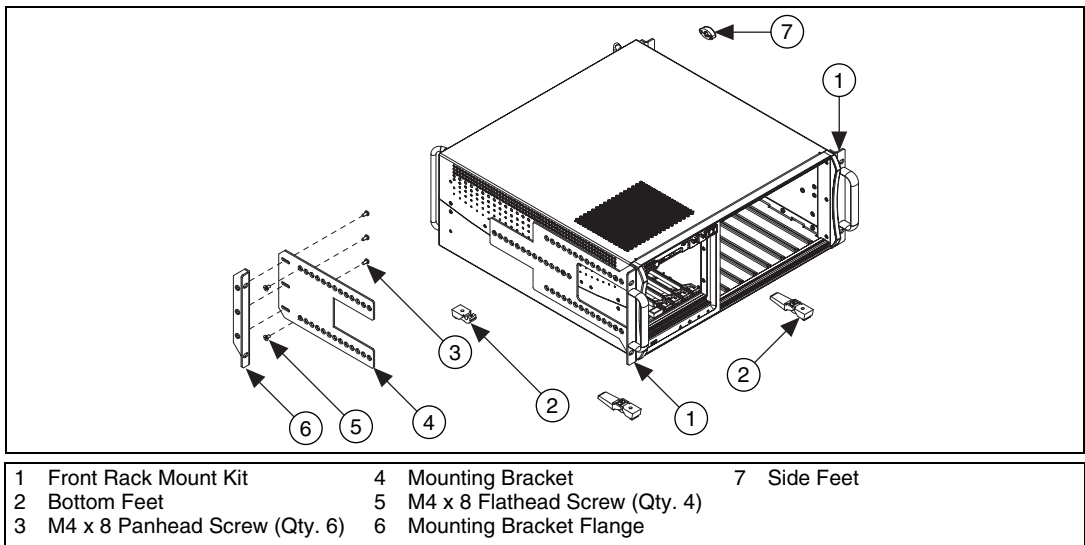


Figure 1. NI PXI-1052 in Rack Mount Configuration

1. Remove the side feet and bottom feet (as required) from the NI PXI-1052 chassis.
2. Install the mounting brackets onto each side of the chassis using the M4 × 8 flathead screws supplied. Notice that you can recess the chassis in the cabinet rack at .5 in. increments.
3. Attach the mounting bracket flanges to the mounting brackets using the M4 × 8 panhead screws supplied.
4. Install the chassis in the instrument rack using eight screws (not supplied).

National Instruments™, NI™, and ni.com™ are trademarks of National Instruments Corporation. Product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products, refer to the appropriate location: **Help» Patents** in your software, the `patents.txt` file on your CD, or ni.com/patents.

© 2004 National Instruments Corp. All rights reserved.



371037A-01

Apr04