

## COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

## SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash    Get Credit    Receive a Trade-In Deal

## OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New, New Surplus, Refurbished, and Reconditioned** NI Hardware.



*Bridging the gap between the manufacturer and your legacy test system.*

 1-800-915-6216

 [www.apexwaves.com](http://www.apexwaves.com)

 [sales@apexwaves.com](mailto:sales@apexwaves.com)

*All trademarks, brands, and brand names are the property of their respective owners.*

**Request a Quote**

 **CLICK HERE**

**PXIe-4309**

# SPECIFICATIONS

# PXIe-4309

32 Ch (8 ADC), 2 MS/s, 18 - 28 bit, Flexible Resolution PXI Analog Input Module

[Français](#)   [Deutsch](#)   [日本語](#)   [한국어](#)   [简体中文](#)

[ni.com/manuals](http://ni.com/manuals)

This document lists specifications for the PXIe-4309 data acquisition module. All specifications are subject to change without notice. Refer to [ni.com/manuals](http://ni.com/manuals) for the most current specifications and product documentation.



**Note** To maintain forced air cooling in the PXIe system, refer to the *Maintain Forced-Air Cooling Note to Users*.

## Terminology

*Maximum* and *minimum* specifications characterize the warranted performance of the instrument within the recommended calibration interval and under the stated operating conditions. These specifications are subject to production verification or guaranteed by design.

*Typical* specifications are specifications met by the majority of the instruments within the recommended calibration interval and under the stated operating conditions, based on measurements taken during production verification and/or engineering development. The performance of the instrument is not warranted.

*Supplemental* specifications describe the basic function and attributes of the instrument established by design and are not subject to production verification. They provide information that is relevant for the adequate use of the instrument that is not included in the previous definitions.

The following specifications are typical at 25 °C, unless otherwise noted.

- $T_{extcal}$  is the device temperature at last external calibration.
- $T_{selfcal}$  is the device temperature at last self-calibration.

# Input Characteristics

---

Number of ADCs .....	8 simultaneously sampling ADCs
Number of channels	
Single channel per ADC .....	8 differential analog input channels
Multichannel per ADC <sup>1</sup> .....	32 differential analog input channels
ADC resolution.....	18 bits
Type of ADC .....	SAR
DNL.....	No missing codes
INL .....	Refer to <i>Absolute Accuracy</i> section
Measurement resolution <sup>2</sup> .....	18 bits - 28 bits
Maximum sample rate <sup>3, 4</sup>	
Auto zero none	
Single channel per ADC .....	2 MS/s
Multichannel per ADC .....	400 kS/s (aggregate)
Auto zero once	
Single channel per ADC .....	2 MS/s
Multichannel per ADC .....	400 kS/s (aggregate)
Auto zero every sample	
Single channel per ADC.....	10 kS/s
Multichannel per ADC .....	10 kS/s (aggregate)
Chopping	
Single channel per ADC.....	10 kS/s
Multichannel per ADC .....	10 kS/s (aggregate)
Input coupling .....	DC
Input range.....	±0.1 V, ±1.0 V, ±10 V, ±15 V
Input overrange .....	0.5% of range
Maximum working voltage (signal + common mode) .....	±15.5 V of GND

---

<sup>1</sup> Up to 4 channels per ADC.

<sup>2</sup> Depends on the sample rate. Refer to the *Noise versus Sampling Rate* section for more information.

<sup>3</sup> For multichannel, up to 4 channels per ADC.

<sup>4</sup> Refer to the *PXIe-4309 User Manual* for Maximum Sample Rates in Hardware-Timed Single Point, On-Demand, and External Sample Clock modes.

## Input impedance

### Device on, channel idle

AI+ to AI- ..... >10 G $\Omega$  in parallel with 100 pF

AI- to GND..... >100 G $\Omega$  in parallel with 10 pF

### Device on, channel active

AI+ to AI- ..... >10 G $\Omega$  in parallel with 200 pF

AI- to GND..... >100 G $\Omega$  in parallel with 100 pF

## Input bias current

Device on, channel active .....  $\pm 4.5$  nA

## Overvoltage protection

Device on/off.....  $\pm 30$  V min

## Overvoltage protection input current

Device on .....  $\pm 100$   $\mu$ A

Device off.....  $\pm 10$   $\mu$ A

FIFO buffer size..... 1,023 samples

Data transfers..... Direct memory access (DMA),  
programmed I/O

# Absolute Accuracy

## Auto Zero None

**Table 1.** DC Voltage Specifications for Auto Zero None

Range	Absolute Accuracy <sup>*, **, ††</sup>			Temperature Coefficient <sup>††</sup>
	24 Hour <sup>†, ‡</sup> T <sub>extcal</sub> ± 1 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 5 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 10 °C T <sub>selfcal</sub> ± 5 °C	0 °C - 55 °C
Range	± (ppm of reading + μV)			± (ppm of reading + μV) / °C
0.1 V	33 + 3.2	60 + 7.6	165 + 11.6	25 + 1
1.0 V	28 + 7.4	55 + 16.2	140 + 36.2	20 + 5
10 V	23 + 59.6	50 + 155	115 + 355	15 + 50
15 V	28 + 89.0	55 + 307	140 + 607	20 + 75

<sup>\*</sup>Source Impedance ≤50 Ω.  
<sup>†</sup>Relative to External Calibration Source.  
<sup>‡</sup>Assumes Offset Nulling.  
<sup>\*\*</sup>Sample Rate ≤10 S/s.  
<sup>††</sup>Temperature Coefficient is an adder to the Absolute Accuracy values that does not apply unless operating outside of the stated self-calibration temperature intervals. Temperature Coefficient is included in the Absolute Accuracy values over the stated self-calibration temperature intervals.

**Table 2.** DC Voltage Performance Specifications for Auto Zero None

Range	Residual Offset <sup>†, ‡</sup> μV	Linearity <sup>†</sup> ppm of range	Noise <sup>*, †, ‡</sup>		
			10 S/s μV <sub>pk-pk</sub>	10 kS/s	2 MS/s μV <sub>rms</sub>
0.1 V	5	5	2.2	0.6	6.9
1.0 V			2.4	0.8	11
10 V			9.6	5.8	84
15 V	75	10	14	8.7	125

<sup>\*</sup>Source Impedance ≤50 Ω.  
<sup>†</sup>Residual Offset, Linearity and Noise are included in the Absolute Accuracy values in the DC voltage specifications table for Sample Rate ≤10 S/s.  
<sup>‡</sup>Noise for Single Channel per ADC. For Multiple Channel per ADC refer to the [Noise versus Sampling Rate](#) section.

# Auto Zero Once

**Table 3.** DC Voltage Specifications for Auto Zero Once

Range	Absolute Accuracy <sup>*, **, ††</sup>			Temperature Coefficient <sup>††</sup>
	24 Hour <sup>†, ‡</sup> T <sub>extcal</sub> ± 1 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 5 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 10 °C T <sub>selfcal</sub> ± 5 °C	0 °C - 55 °C
	± (ppm of reading + μV)			± (ppm of reading + μV) / °C
0.1 V	33 + 2.3	60 + 6.7	165 + 7.1	25 + 0.1
1.0 V	28 + 2.5	55 + 11.3	140 + 11.7	20 + 0.1
10 V	23 + 9.7	50 + 104.9	115 + 105.3	15 + 0.1
15 V	28 + 14.1	55 + 232.1	140 + 232.5	20 + 0.1

\*Source Impedance ≤50 Ω.  
†Relative to External Calibration Source.  
‡Assumes Offset Nulling.  
\*\*Sample Rate ≤10 S/s.  
††Temperature Coefficient is an adder to the Absolute Accuracy values that does not apply unless operating outside of the stated self-calibration temperature intervals. Temperature Coefficient is included in the Absolute Accuracy values over the stated self-calibration temperature intervals.

**Table 4.** DC Voltage Performance Specifications for Auto Zero Once

Range	Residual Offset <sup>*, †</sup>	Linearity <sup>†</sup>	Noise <sup>*, †, ‡</sup>		
			10 S/s	10 kS/s	2 MS/s
	μV	ppm of range	μV <sub>pk-pk</sub>	μV <sub>rms</sub>	
0.1 V	5	5	2.2	0.6	6.9
1.0 V			2.4	0.8	11
10 V	50		9.6	5.8	84
15 V	75	10	14	8.7	125

\*Source Impedance ≤50 Ω.  
†Residual Offset, Linearity and Noise are included in the Absolute Accuracy values in the DC voltage specifications table for Sample Rate ≤10 S/s.  
‡Noise for Single Channel per ADC. For Multiple Channel per ADC refer to the [Noise versus Sampling Rate](#) section.

# Auto Zero Every Sample

**Table 5.** DC Voltage Specifications for Auto Zero Every Sample

Range	Absolute Accuracy <sup>*, **, ††</sup>			Temperature Coefficient <sup>††</sup>
	24 Hour <sup>†, ‡</sup> T <sub>extcal</sub> ± 1 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 5 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 10 °C T <sub>selfcal</sub> ± 5 °C	0 °C - 55 °C
	± (ppm of reading + μV)			± (ppm of reading + μV) / °C
0.1 V	33 + 0.3	60 + 4.7	165 + 5.1	25 + 0.1
1.0 V	28 + 0.5	55 + 9.3	140 + 9.7	20 + 0.1
10 V	23 + 2.7	50 + 55.4	115 + 55.8	15 + 0.1
15 V	28 + 4.0	55 + 156.1	140 + 156.5	20 + 0.1

<sup>\*</sup>Source Impedance ≤50 Ω.  
<sup>†</sup>Relative to External Calibration Source.  
<sup>‡</sup>Assumes Offset Nulling.  
<sup>\*\*</sup>Sample Rate ≤10 S/s.  
<sup>††</sup>Temperature Coefficient is an adder to the Absolute Accuracy values that does not apply unless operating outside of the stated self-calibration temperature intervals. Temperature Coefficient is included in the Absolute Accuracy values over the stated self-calibration temperature intervals.

**Table 6.** DC Voltage Performance Specification for Auto Zero Every Sample

Range	Residual Offset <sup>*, †</sup>	Linearity <sup>†</sup>	Noise <sup>*, †, ‡</sup>	
			10 S/s	10 kS/s
	μV	ppm of range	μV <sub>pk-pk</sub>	μV <sub>rms</sub>
0.1 V	4	5	0.2	0.8
1.0 V			0.4	1.1
10 V			2.6	7.4
15 V		10	3.9	11

<sup>\*</sup>Source Impedance ≤50 Ω.  
<sup>†</sup>Residual Offset, Linearity and Noise are included in the Absolute Accuracy values in the DC voltage specifications table for Sample Rate ≤10 S/s.  
<sup>‡</sup>Noise for Single Channel per ADC. For Multiple Channel per ADC refer to the *Noise versus Sampling Rate* section.

# Chopping

**Table 7. DC Voltage Specifications for Chopping**

Range	Absolute Accuracy <sup>*, **, ††</sup>			Temperature Coefficient <sup>††</sup>
	24 Hour <sup>†, ‡</sup> T <sub>extcal</sub> ± 1 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 5 °C T <sub>selfcal</sub> ± 1 °C	2 Year T <sub>extcal</sub> ± 10 °C T <sub>selfcal</sub> ± 5 °C	0 °C - 55 °C
	± (ppm of reading + μV)			± (ppm of reading + μV) / °C
0.1 V	33 + 0.1	60 + 2.6	165 + 2.6	25 + 0.01
1.0 V	28 + 0.2	55 + 7.1	140 + 7.2	20 + 0.01
10 V	23 + 1.3	50 + 52.7	115 + 52.7	15 + 0.01
15 V	28 + 2.0	55 + 153.0	140 + 153.1	20 + 0.01

<sup>\*</sup>Source Impedance ≤ 50 Ω.  
<sup>†</sup>Relative to External Calibration Source.  
<sup>‡</sup>Assumes Offset Nulling.  
<sup>\*\*</sup>Sample Rate ≤ 10 S/s.  
<sup>††</sup>Temperature Coefficient is an adder to the Absolute Accuracy values that does not apply unless operating outside of the stated self-calibration temperature intervals. Temperature Coefficient is included in the Absolute Accuracy values over the stated self-calibration temperature intervals.

**Table 8. DC Voltage Performance Specifications for Chopping**

Range	Residual Offset <sup>*, †</sup>	Linearity <sup>†</sup>	Noise <sup>*, †, ‡</sup>	
			10 S/s	10 kS/s
	μV	ppm of range	μV <sub>pk-pk</sub>	μV <sub>rms</sub>
0.1 V	2	5	0.1	0.5
1.0 V			0.2	0.8
10 V			1.3	6.2
15 V		10	2	9.2

<sup>\*</sup>Source Impedance ≤ 50 Ω.  
<sup>†</sup>Residual Offset, Linearity and Noise are included in the Absolute Accuracy values in the DC voltage specifications table for Sample Rate ≤ 10 S/s.  
<sup>‡</sup>Noise for Single Channel per ADC. For Multiple Channel per ADC refer to the [Noise versus Sampling Rate](#) section.



# Offset Cancellation Long Term Stability Performance


TB-4309 (ST), analog inputs shorted at the terminal block screw terminals

Continuous Acquisition, 0.1 V Range, Auto Zero Every Sample, 2 S/s

Offset Nulling: 2 samples prior to continuous acquisition


Waveform Filter: Average and Decimate by 720 (10 S/hr)

**Figure 1.** Auto Zero Every Sample Offset Cancellation Stability

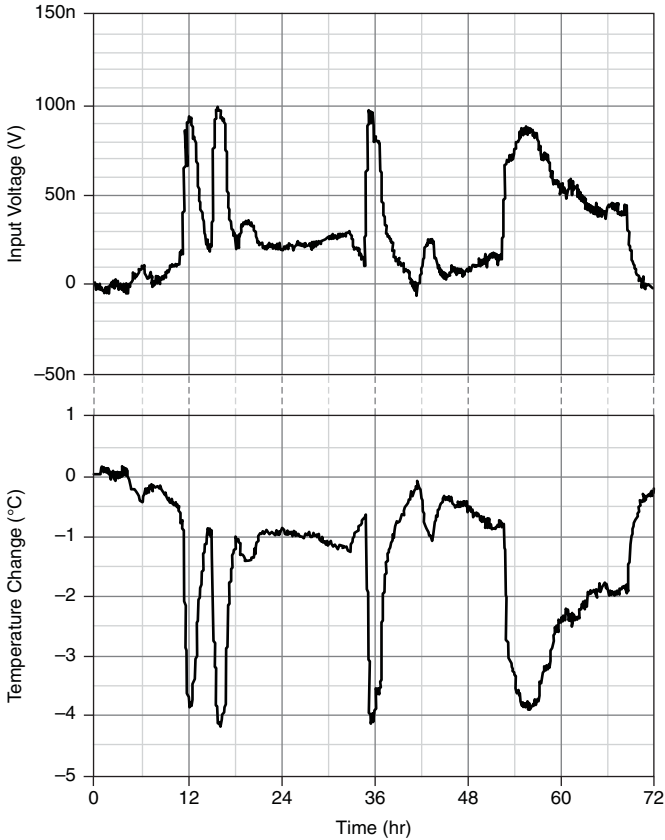

TB-4309 (ST), analog inputs shorted at the terminal block screw terminals  
Continuous Acquisition, 0.1 V Range, Chopping, 2 S/s  
Offset Nulling: 2 samples prior to continuous acquisition  
Waveform Filter: Average and Decimate by 720 (10 S/hr)


**Figure 2.** Chopping Offset Cancellation Stability

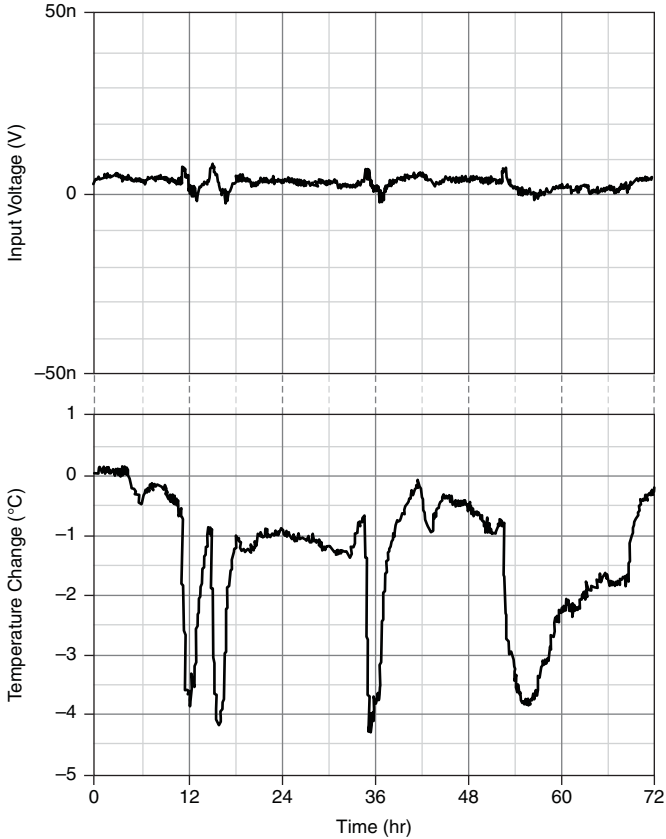

# Offset Cancellation Spectral Noise Density Performance

TB-4309 (ST), analog inputs shorted at the terminal block screw terminals  
Continuous Acquisition, 0.1 V Range, 518400 Samples acquired at 2 S/s


**Figure 3.** Offset Cancellation Spectral Noise Density

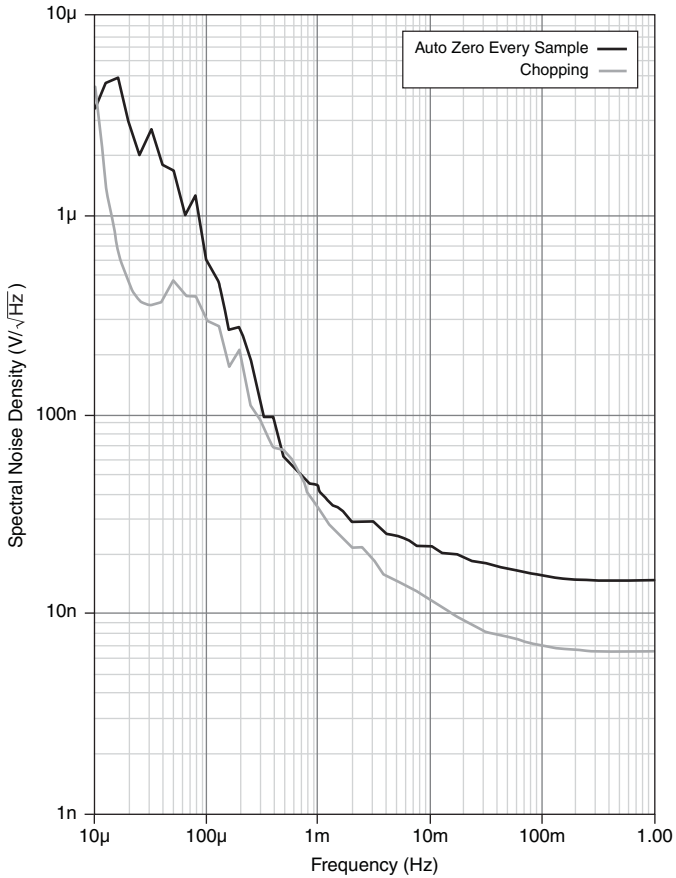


# Noise versus Sampling Rate

## Auto Zero None and Auto Zero Once

**Figure 4.** Noise versus Sample Rate (Single channel per ADC)

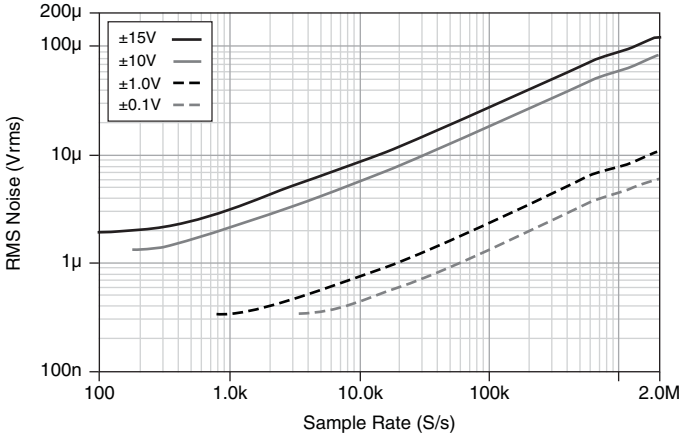


**Figure 5.** Noise versus Sample Rate (Multichannel per ADC)

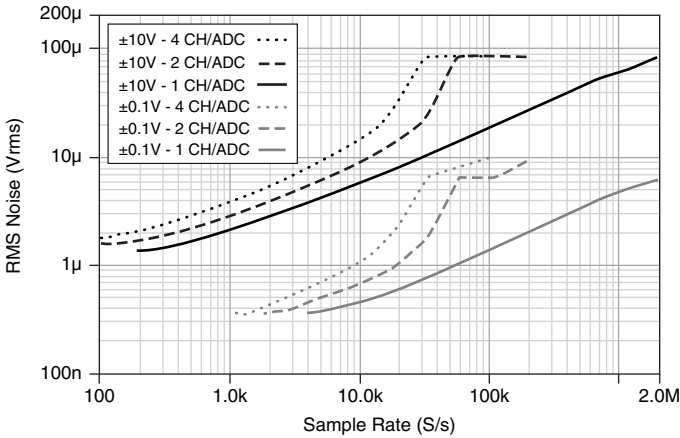


# Auto Zero Every Sample

**Figure 6.** Noise versus Sample Rate (Single channel per ADC)

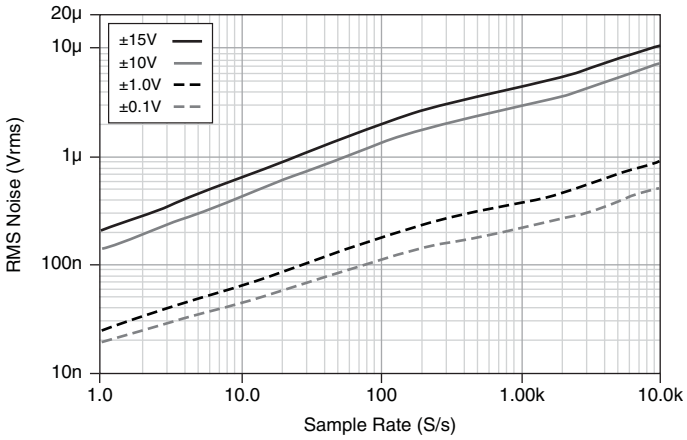


**Figure 7.** Noise versus Sample Rate (Multichannel per ADC)

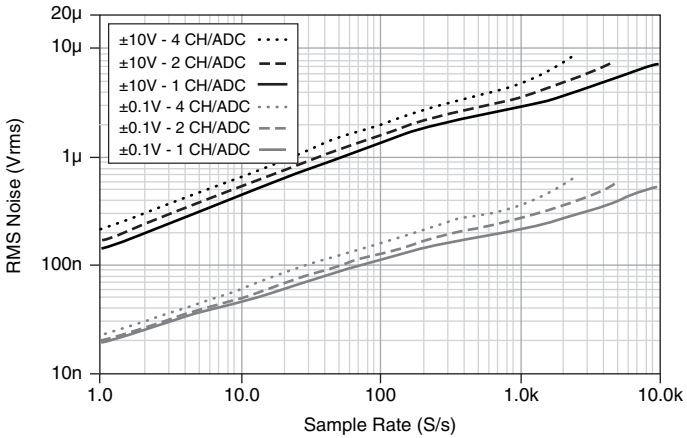


# Chopping

**Figure 8.** Noise versus Sample Rate (Single channel per ADC)

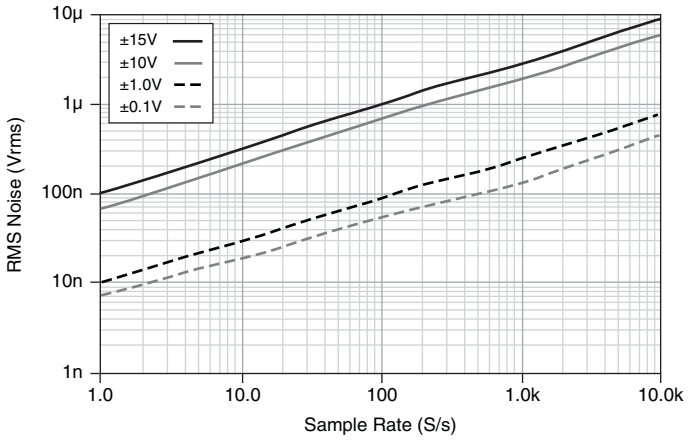

**Figure 9.** Noise versus Sample Rate (Multichannel per ADC)

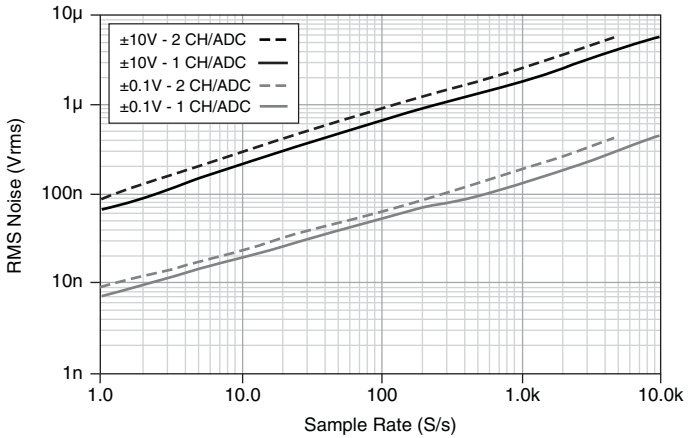


# Digital Filter Frequency Response<sup>1, 2, 3</sup>

---

**Figure 10.** Digital Filter Frequency Response

---

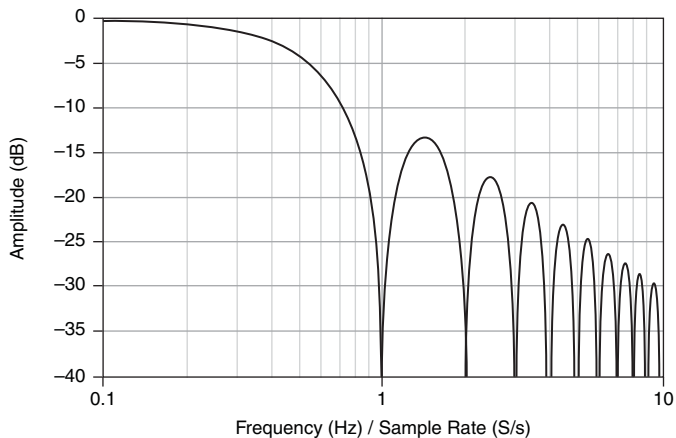

---

<sup>1</sup> Applies to sampling rates  $\leq 1$  MS/s for all configurations that use a single channel per ADC.

<sup>2</sup> Applies to sampling rates  $\leq 200$  kS/s (aggregate) for all configurations that use multiple channels per ADC.

<sup>3</sup> Does not apply to Hardware-Timed Single Point, On-Demand, and External Sample Clock modes.

# Dynamic Characteristics

## Spectral Noise Density


Input voltage noise density at 1 kHz

0.1 V .....	6.2 nV/ $\sqrt{\text{Hz}}$
1.0 V .....	12 nV/ $\sqrt{\text{Hz}}$
10 V .....	94 nV/ $\sqrt{\text{Hz}}$
15 V .....	136 nV/ $\sqrt{\text{Hz}}$

Input current noise density at 1 kHz..... 0.5 pA/ $\sqrt{\text{Hz}}$


## Auto Zero None and Auto Zero Once

**Figure 11.** 2 MS/s Spectral Noise Density (Single channel per ADC)

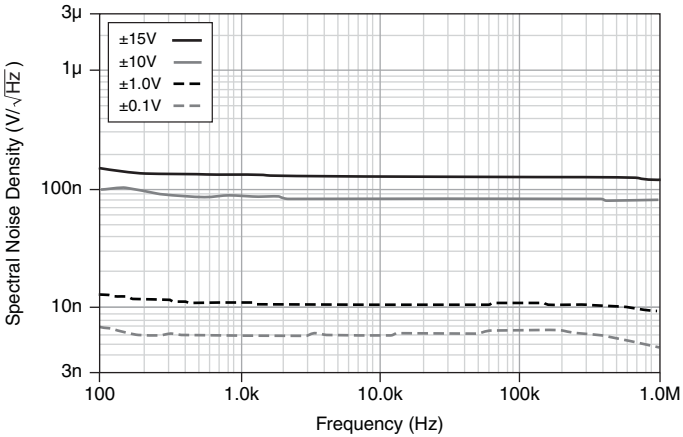





**Figure 12.** 20 kS/s Spectral Noise Density (Single channel per ADC)

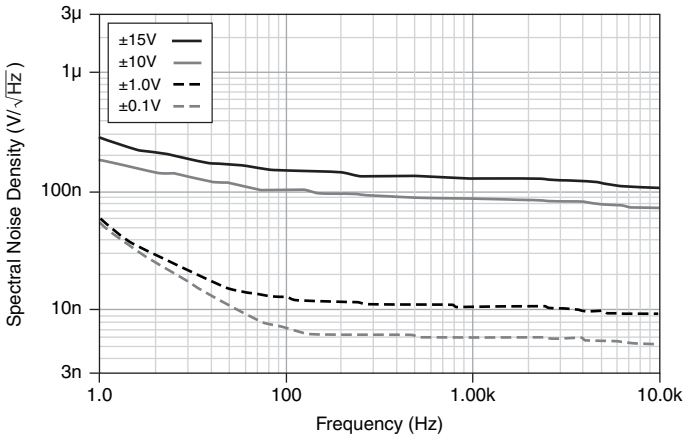


**Figure 13.** 20 kS/s Spectral Noise Density (Multichannel per ADC)

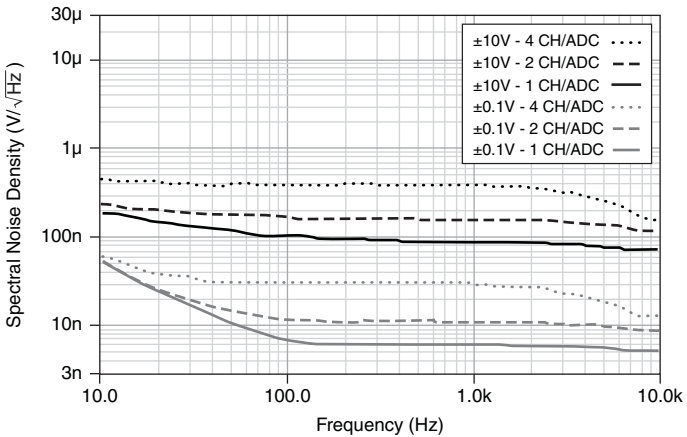

**Figure 14.** 2 kS/s Spectral Noise Density (Single channel per ADC)

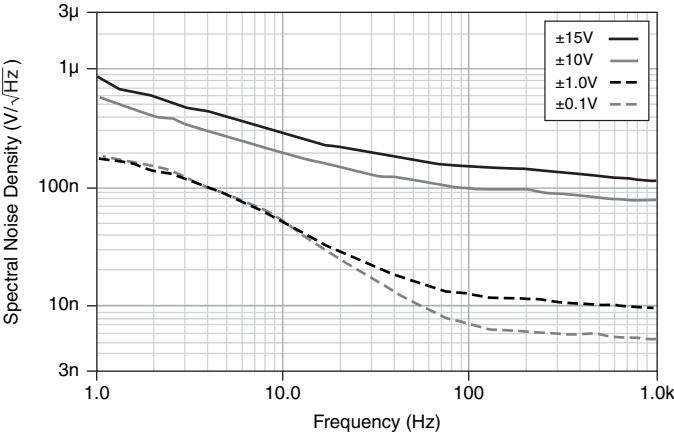


**Figure 15.** 2 kS/s Spectral Noise Density (Multichannel per ADC)

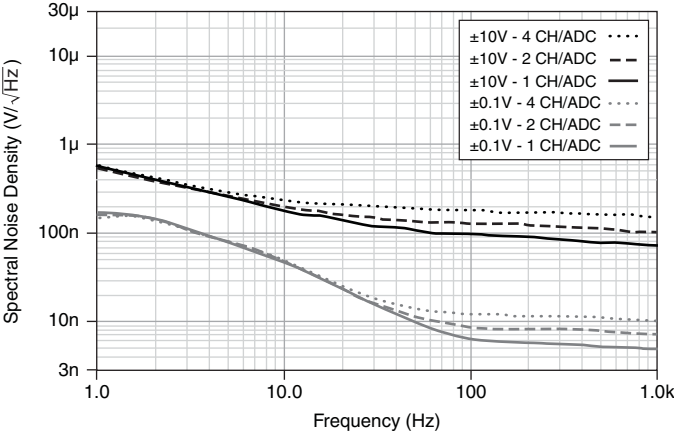


# Auto Zero Every Sample

**Figure 16.** 2 kS/s Spectral Noise Density (Single channel per ADC)

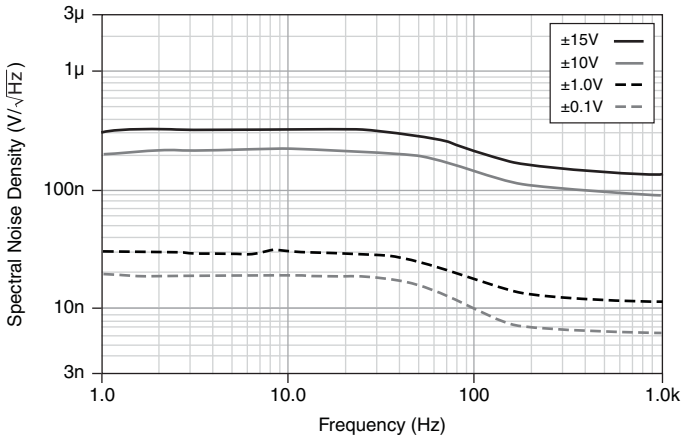


**Figure 17.** 2 kS/s Spectral Noise Density (Multichannel per ADC)

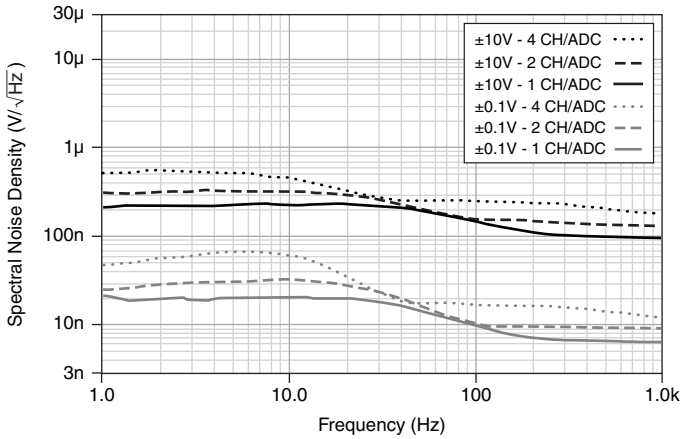


# Chopping

**Figure 18.** 2 kS/s Spectral Noise Density (Single channel per ADC)

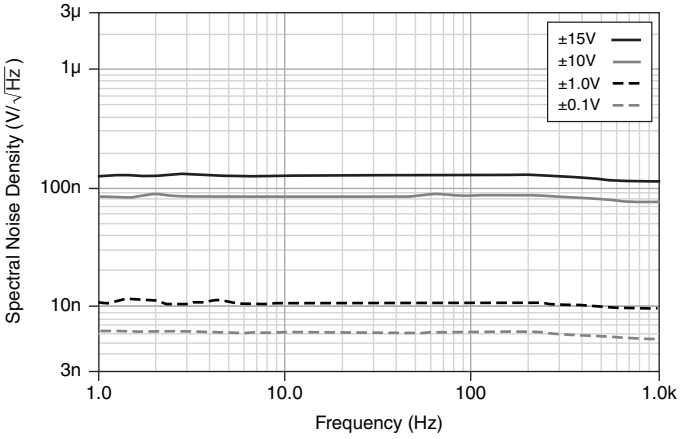


**Figure 19.** 2 kS/s Spectral Noise Density (Multichannel per ADC)

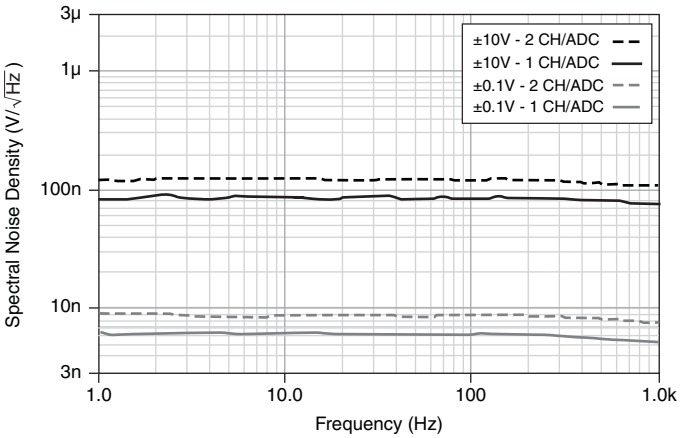

# Common-Mode Rejection Ratio (CMRR)

DC.....	>160 dBc
DC - 100 Hz	
0.1 V, 1.0 V .....	>126 dBc
10 V.....	>120 dBc
15 V.....	>114 dBc

**Figure 20.** Common-Mode Rejection Ratio

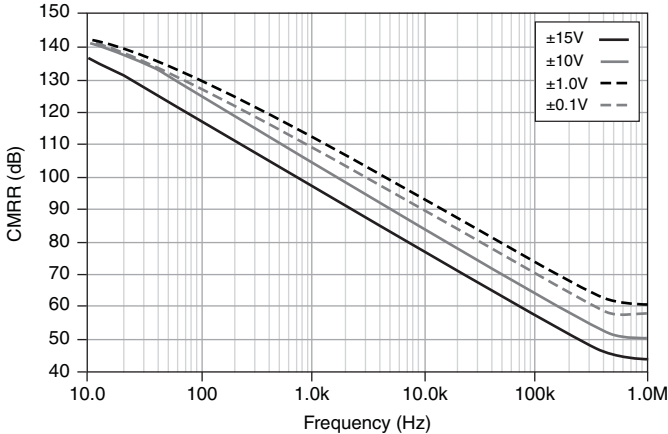

## Crosstalk, Input Channel Separation<sup>1</sup>

TB-4309 (ST)<sup>2</sup> and TB-4309 (MT)<sup>3</sup>

1 kHz.....	Typically ≤ -120 dBc
10 kHz.....	Typically ≤ -100 dBc
100 kHz.....	Typically ≤ -80 dBc
500 kHz.....	Typically ≤ -70 dBc

<sup>1</sup> To maintain crosstalk performance use separation and/or shielding between signal cables.


<sup>2</sup> Inputs shorted at terminal block screw terminals.

<sup>3</sup> Inputs shorted at SCB-68 screw terminals using 2 m, 68-pin cable.

# Bandwidth

-3.0 dB bandwidth ..... 500 kHz

**Figure 21. Magnitude Response**

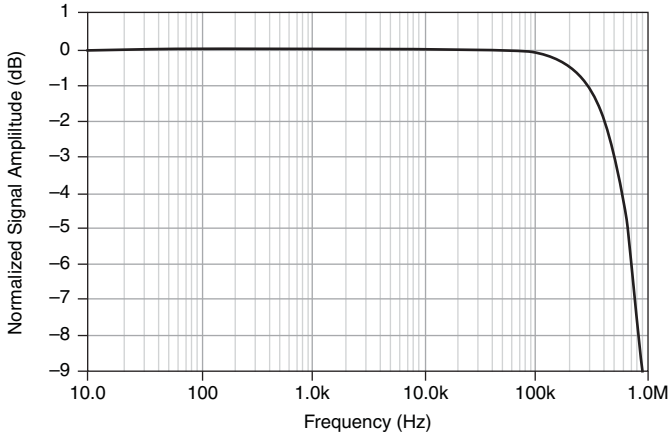


# Flatness

DC - 20 kHz ..... -6.5 mdB


DC - 80 kHz ..... -100 mdB

**Figure 22. Flatness**

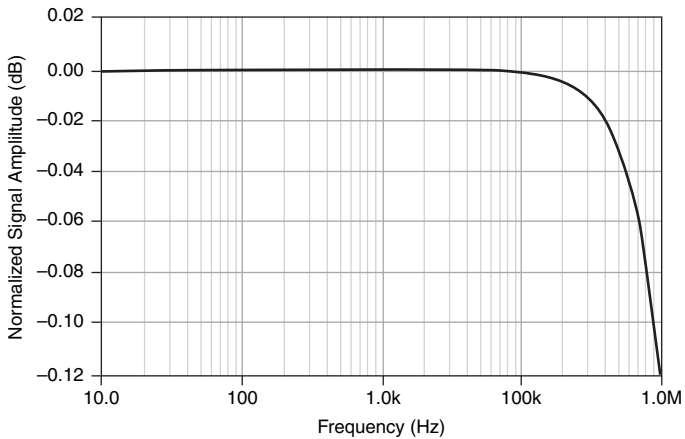


# Source Impedance Error

**Figure 23.** Source Impedance Reading Error<sup>1</sup>

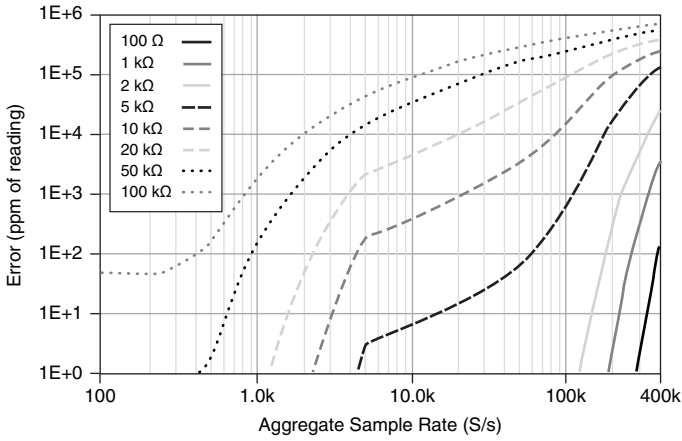

**Figure 24.** Source Impedance Ghosting Error<sup>2</sup>

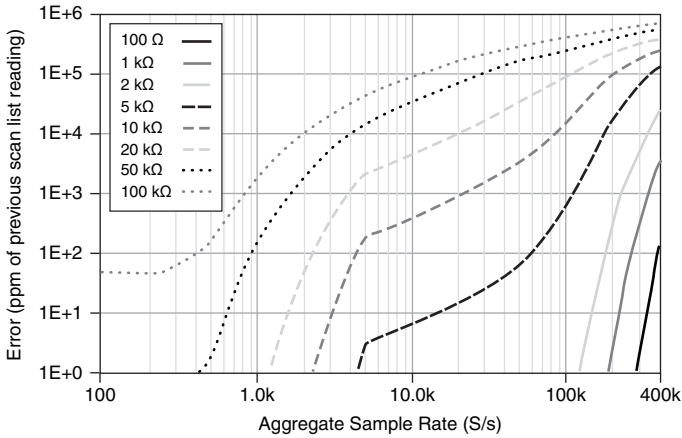

<sup>1</sup> Applies to all configurations that use multiple channels per ADC, Auto Zero Every Sample or Chopping.

<sup>2</sup> Applies to all configurations that use multiple channels per ADC.

# Onboard Calibration Reference

---

## Voltage

Output voltage range .....	6.741 V – 7.298 V
Output current drive .....	±1 $\mu$ A
Temperature coefficient .....	±1 ppm/°C
Overvoltage protection .....	±30 V min

## Frequency Timebase Characteristics

Resolution .....	10 ns
Accuracy	
Using internal timebase .....	±50 ppm
Using external timebase .....	Equal to accuracy of external timebase

## Timing and Synchronization

---

Number of timing engines .....	1
Reference clock source .....	Onboard clock, backplane PXIe_CLK100

## Digital Triggers

Purpose .....	Start trigger, reference trigger, pause trigger
Source .....	PFI 0, PFI 1, PXI_Trig <0..7>, PXI_Star, PXIe_DStar A, PXIe_DStar B
Polarity .....	Software-selectable
Debounce filter settings .....	Disable, 90 ns, 5.12 $\mu$ s, custom interval

## Output Timing Signals

Source .....	Start trigger, reference trigger, pause trigger, sample clock
Destination .....	PFI 0, PFI 1, PXI_Trig <0..7>, PXIe_DStarC



# PFI 0 and PFI 1 (Front Panel Digital Triggers)

## Input

Logic compatibility.....	3.3 V or 5 V
High, VIH.....	2.40 V min
Low, VIL.....	0.95 V max
Input impedance.....	10 k $\Omega$
Input current ( $0\text{ V} \leq V_{in} \leq 5\text{ V}$ ).....	$\leq 500\ \mu\text{A}$
Overvoltage protection.....	$\pm 30\text{ V min}$

## Output

High, VOH.....	3.43 V max
Sourcing 5 mA.....	2.88 V min
Low, VOL.....	
Sinking 5 mA.....	0.33 V max
Output impedance.....	50 $\Omega$
Output current.....	$\pm 30\text{ mA min}$
Overvoltage protection.....	$\pm 30\text{ V min}$

# General Specifications

---

## Bus Interface

Form factor.....	x1 PXI Express peripheral module, specification rev 1.0 compliant
Slot compatibility.....	PXI Express or PXI Express hybrid slots
DMA channels.....	1, analog input

## Power Requirements

+12 V.....	2 A max
+3.3 V.....	1 A max

# Physical

Dimensions.....	16 cm × 10 cm (6.3 in. × 3.9 in.) 3U CompactPCI slot
Weight .....	238 g (8.4 oz)
I/O connector.....	96-pin male DIN 41612/IEC 60603-2 connector
Measurement Category <sup>1</sup> .....	I



**Caution** Do *not* use the PXIe-4309 for connections to signals or for measurements within Categories II, III, or IV.



**Caution** The protection provided by the PXIe-4309 can be impaired if it is used in a manner not described in this document.



**Caution** Clean the hardware with a soft, nonmetallic brush. Make sure that the hardware is completely dry and free from contaminants before returning it to service.

# Environmental Specifications

---

## Operating Environment

Ambient temperature range.....	0 °C to 55 °C (Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 low temperature limit and MIL-PRF-28800F Class 2 high temperature limit.)
Relative humidity range .....	10% to 90%, noncondensing (Tested in accordance with IEC 60068-2-56.)
Maximum altitude.....	2,000 m (800 mbar)
Pollution Degree .....	2

Indoor use only.

---

<sup>1</sup> Measurement Categories CAT I and CAT O are equivalent. These test and measurement circuits are not intended for direct connections to the MAINS building installations of Measurement Categories CAT II, CAT III, CAT IV.

# Storage Environment

Ambient temperature range .....	-40 °C to 71 °C (Tested in accordance with IEC 60068-2-1 and IEC 60068-2-2. Meets MIL-PRF-28800F Class 3 limits.)
Relative humidity range .....	5% to 95%, noncondensing (Tested in accordance with IEC 60068-2-56.)

# Shock and Vibration

---

Operating shock.....	30 g peak, half-sine, 11 ms pulse (Tested in accordance with IEC 60068-2-27. Meets MIL-PRF-28800F Class 2 limits.)
Random vibration	
Operating.....	5 Hz to 500 Hz, 0.3 grms
Non-operating.....	5 Hz to 500 Hz, 2.4 grms (Tested in accordance with IEC 60068-2-64. Non-operating test profile exceeds the requirements of MIL-PRF-28800F, Class 3.)

# Calibration

---

You can obtain the calibration certificate and information about calibration services for the PXIe-4309 at [ni.com/calibration](http://ni.com/calibration).

Self-calibration.....	On software command, the module computes gain, offset, and linearity corrections relative to the high-precision internal voltage reference.
Self-calibration interval .....	Depending on required absolute accuracy, self-calibration is recommended whenever the current device temperature differs by more than the specified temperature range from the device temperature at which the last self-calibration was performed.
Calibration interval.....	2 years
Warm-up time.....	15 minutes

# Safety

---

This product meets the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1



**Note** For UL and other safety certifications, refer to the product label or the [Online Product Certification](#) section.

# Electromagnetic Compatibility

---

This product meets the requirements of the following EMC standards for electrical equipment for measurement, control, and laboratory use:

- EN 61326-1 (IEC 61326-1): Class A emissions; Basic immunity
- EN 55011 (CISPR 11): Group 1, Class A emissions
- EN 55022 (CISPR 22): Class A emissions
- EN 55024 (CISPR 24): Immunity
- AS/NZS CISPR 11: Group 1, Class A emissions
- AS/NZS CISPR 22: Class A emissions
- FCC 47 CFR Part 15B: Class A emissions
- ICES-001: Class A emissions



**Note** In the United States (per FCC 47 CFR), Class A equipment is intended for use in commercial, light-industrial, and heavy-industrial locations. In Europe, Canada, Australia and New Zealand (per CISPR 11) Class A equipment is intended for use only in heavy-industrial locations.



**Note** Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generate radio frequency energy for the treatment of material or inspection/analysis purposes.



**Note** For EMC declarations and certifications, and additional information, refer to the [Online Product Certification](#) section.



**Note** Group 1 equipment (per CISPR 11) is any industrial, scientific, or medical equipment that does not intentionally generate radio frequency energy for the treatment of material or inspection/analysis purposes.



**Note** For EMC declarations and certifications, and additional information, refer to the [Online Product Certification](#) section.

# CE Compliance

---

This product meets the essential requirements of applicable European Directives as follows:

- 2014/35/EU; Low-Voltage Directive (safety)
- 2014/30/EU; Electromagnetic Compatibility Directive (EMC)

## Online Product Certification

---

Refer to the product Declaration of Conformity (DoC) for additional regulatory compliance information. To obtain product certifications and the DoC for this product, visit [ni.com/certification](https://ni.com/certification), search by model number or product line, and click the appropriate link in the Certification column.

## Environmental Management

---

NI is committed to designing and manufacturing products in an environmentally responsible manner. NI recognizes that eliminating certain hazardous substances from our products is beneficial to the environment and to NI customers.

For additional environmental information, refer to the *Minimize Our Environmental Impact* web page at [ni.com/environment](https://ni.com/environment). This page contains the environmental regulations and directives with which NI complies, as well as other environmental information not included in this document.

## Waste Electrical and Electronic Equipment (WEEE)



**EU Customers** At the end of the product life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers, National Instruments WEEE initiatives, and compliance with WEEE Directive 2002/96/EC on Waste and Electronic Equipment, visit [ni.com/environment/weee](https://ni.com/environment/weee).

## 电子信息产品污染控制管理办法（中国 RoHS）



**中国客户** National Instruments 符合中国电子信息产品中限制使用某些有害物质指令 (RoHS)。关于 National Instruments 中国 RoHS 合规性信息，请登录 [ni.com/environment/rohs\\_china](https://ni.com/environment/rohs_china)。(For information about China RoHS compliance, go to [ni.com/environment/rohs\\_china](https://ni.com/environment/rohs_china).)

# Worldwide Support and Services

---

The NI website is your complete resource for technical support. At [ni.com/support](http://ni.com/support) you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit [ni.com/services](http://ni.com/services) for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit [ni.com/register](http://ni.com/register) to register your NI product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

A Declaration of Conformity (DoC) is our claim of compliance with the Council of the European Communities using the manufacturer's declaration of conformity. This system affords the user protection for electromagnetic compatibility (EMC) and product safety. You can obtain the DoC for your product by visiting [ni.com/certification](http://ni.com/certification). If your product supports calibration, you can obtain the calibration certificate for your product at [ni.com/calibration](http://ni.com/calibration).

NI corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. NI also has offices located around the world. For telephone support in the United States, create your service request at [ni.com/support](http://ni.com/support) or dial 1 866 ASK MYNI (275 6964). For telephone support outside the United States, visit the Worldwide Offices section of [ni.com/niglobal](http://ni.com/niglobal) to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.

Refer to the *NI Trademarks and Logo Guidelines* at [ni.com/trademarks](http://ni.com/trademarks) for more information on NI trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering NI products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at [ni.com/patents](http://ni.com/patents). You can find information about end-user license agreements (EULAs) and third-party legal notices in the `readme` file for your NI product. Refer to the *Export Compliance Information* at [ni.com/legal/export-compliance](http://ni.com/legal/export-compliance) for the NI global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2017 National Instruments. All rights reserved.