

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

PXIe-8105

CALIBRATION PROCEDURE

PXIe-5665

3.6 GHz and 14 GHz RF Vector Signal Analyzer

This document contains the verification procedures for the National Instruments PXIe-5665 RF vector signal analyzer (VSA). Refer to ni.com/calibration for more information about calibration solutions.

When not otherwise specified, the procedures in this document refer to both the PXIe-5665 3.6 GHz VSA and the PXIe-5665 14 GHz VSA products. In places where the procedures differ between the two products, the appropriate device settings are specified.



Note PXIe-5665 tuned frequencies greater than 3.6 GHz and procedures with the preselector enabled for frequencies greater than 3.6 GHz apply only to the PXIe-5665 14 GHz VSA.

NI warrants the PXIe-5665 to meet its published specifications if the individual modules are calibrated and operating within specifications. For more information about RF system calibration, visit ni.com/manuals and search for Letter of Conformance.

Contents

Software.....	2
Documentation.....	2
Test Equipment.....	3
Test Conditions.....	10
System Options.....	11
Initial Setup.....	11
Characterizing the Test System.....	11
Zeroing and Calibrating the Power Sensor.....	11
Characterizing Power Splitter Reference Output.....	11
Characterizing Power Splitter Difference.....	12
Characterizing RF Source Power (Direct).....	13
Characterizing RF Source Power (with Lowpass Filter).....	15
Characterizing RF Source Power (Combined) for Frequencies ≤ 700 MHz.....	17
Characterizing RF Source Power (Combined) for Frequencies > 700 MHz.....	19
Characterizing RF Source Power (Through Splitter).....	21
Characterizing RF Source Power (with Splitter and Attenuator).....	23
Characterizing Spectrum Analyzer Response.....	25
As-Found and As-Left Limits.....	27
Verification.....	27
Verifying Reference Accuracy.....	27
Verifying Phase Noise.....	27

Verifying Frequency Response and Absolute Amplitude Accuracy	28
Verifying Frequency Response and Absolute Amplitude Accuracy for Frequencies >10 MHz	28
Verifying Average Noise Level	35
Verifying Non-Input-Related Spurs (Residual Spurs)	40
Verifying LO-Related Spurs (Sideband Spurs)	43
Verifying Image Rejection	48
Verifying Third-Order Intermodulation Distortion	53
Frequencies \leq 700 MHz	53
Frequencies >700 MHz	57
Verifying Second Harmonic Intercept (SHI)	62
Verifying Gain Compression	67
Frequencies \leq 700 MHz	68
Frequencies >700 MHz	73
Verifying LO Output Power	79
Reverification	83
Appendix A: Anti-Distortion Test Fixture	83
Appendix B: Power Sensor Calibration Factor Uncertainty	84
Worldwide Support and Services	85

Software

Calibrating the PXIe-5665 requires you to install the following software on the calibration system:

- NI-RFSA 2.5 or later
- NI Spectral Measurements Toolkit 2.5 or later

You can download all required software from ni.com/downloads.

The software supports programming the calibration procedures in the LabVIEW, C, and LabWindows™/CVI™ application development environments (ADEs). When you install the software, you need to install support only for the ADE that you intend to use.

Documentation

You might find the following documents helpful as you perform the calibration procedure:

- *NI 5665 RF Vector Signal Analyzer Getting Started Guide*
- *NI RF Vector Signal Analyzers Help*
- *PXIe-5665 Specifications*

The latest versions of these documents are available at ni.com/manuals.

This calibration procedure calibrates the PXIe-5665 as a single system. To calibrate the PXIe-5653 or PXIe-5622 individually, refer to their calibration procedures, available at ni.com/manuals.

Test Equipment

Table 1 lists the equipment NI recommends for the performance verification procedures. If the recommended equipment is not available, select a substitute using the minimum requirements listed in the table.

Table 1. Recommended Equipment for PXIe-5665 Calibration

Equipment	Recommended Models	Where Used	Minimum Requirements
Power meter	Anritsu ML2438A	Verifying frequency response, Verifying absolute amplitude accuracy, Verifying LO output power	Display resolution: ≤ 0.01 dB Settling: $\pm 0.1\%$ Instrumentation accuracy: $\leq \pm 0.5\%$ Noise, zero set, and drift: $\leq \pm 0.5\%$ full-scale (lowest range) Reference power uncertainty: $\leq \pm 0.9\%$ Reference output VSWR: $< 1.04 : 1$
Power sensors (2x)	Anritsu SC7400	Verifying frequency response, Verifying absolute amplitude accuracy, Verifying LO output power	Power range: -55 dBm to 20 dBm Frequency range: 10 MHz to 16 GHz Input VSWR: 10 MHz to 150 MHz $\leq 1.17 : 1$ 150 MHz to 2 GHz $\leq 1.08 : 1$ 2 GHz to 12.4 GHz $\leq 1.16 : 1$ 12.4 GHz to 18 GHz $\leq 1.21 : 1$ Linearity: -55 dBm to 20 dBm $\leq 1.8\%$ Calibration factor uncertainty: Refer to Appendix B: Power Sensor Calibration Factor Uncertainty

Table 1. Recommended Equipment for PXIe-5665 Calibration (Continued)

Equipment	Recommended Models	Where Used	Minimum Requirements
Signal generator (RF source 1)	Anritsu MG3692C Options 2A, 3, 4, 15A, and 22	Verifying third-order intermodulation distortion, Verifying gain compression	Frequency range: 8 MHz to 16 GHz Leveled power: -115 dBm to 18 dBm Power accuracy: ± 1.5 dB Harmonics: 0.1 MHz to ≤ 10 MHz <-30 dBc >10 MHz to ≤ 100 MHz <-40 dBc >100 MHz to ≤ 2.2 GHz <-50 dBc >2.2 GHz to ≤ 16 GHz <-30 dBc Nonharmonic spurious: 0.1 MHz to ≤ 10 MHz <-30 dBc >10 MHz to ≤ 2.2 GHz <-60 dBc >2.2 GHz to ≤ 16 GHz <-60 dBc Output VSWR: <2.0 : 1
Signal generator (RF source 2)	Anritsu MG3692C Options 2A, 3, 4, 15A, and 22	Verifying frequency response, Verifying absolute amplitude accuracy, Verifying LO-related spurs, Verifying image rejection, Verifying third-order intermodulation distortion, Verifying second harmonic intercept, Verifying gain compression, Verifying LO output power	Frequency range: 0.1 Hz to 16 GHz Leveled power: -115 dBm to 18 dBm Power accuracy: ± 1.5 dB Harmonics: 0.1 MHz to ≤ 10 MHz <-30 dBc >10 MHz to ≤ 100 MHz <-40 dBc >100 MHz to ≤ 2.2 GHz <-50 dBc >2.2 GHz to ≤ 16 GHz <-30 dBc Nonharmonic spurious: 0.1 MHz to 10 MHz <-30 dBc 10 MHz to ≤ 2.2 MHz <-60 dBc >2.2 GHz to ≤ 16 GHz <-60 dBc Output VSWR: <2.0 : 1

Table 1. Recommended Equipment for PXIe-5665 Calibration (Continued)

Equipment	Recommended Models	Where Used	Minimum Requirements
Spectrum analyzer	Rohde & Schwarz FSUP26 Options B60 and B61	Verifying frequency response, Verifying phase noise, Verifying LO-related spurs, Verifying LO output power	Frequency range: 10 MHz to 18 GHz Noise floor: <-152 dBm/Hz Phase noise measurement using cross-correlation Frequency counter marker feature Spectrum analysis capabilities
50 Ω termination (three are included in the PXIe-5665 kit)	NI 778353-01	Verifying average noise level, Verifying non-input-related (residual) spurs	—
PXI Express chassis	PXIe-1065 or PXIe-1075	—	—
PXI Express controller	PXIe-8105 or PXIe-8133	—	—
SMA (m)-to- SMA (m) semi-rigid cables (3x)*	NI 151611A-01	—	—
SMA (m)-to- SMA (m) semi-rigid cable*	NI 151612A-01	—	—
SMA (m)-to- SMA (m) semi-flexible cable*	NI 190412B-04	—	—
SMA (m)-to- SMA (m) flexible cable*	NI 151890A-1R25	—	—

Table 1. Recommended Equipment for PXIe-5665 Calibration (Continued)

Equipment	Recommended Models	Where Used	Minimum Requirements
SMA (m)-to-SMA (m) cables (36 in.) (3x)	MegaPhase G916-SISI-36	—	Frequency range: DC to 18 GHz Insertion loss: ≤ 2 dB at 18 GHz Impedance: 50 Ω VSWR: $\leq 1.35 : 1$ at 18 GHz
3.5 mm (m)-to-3.5 mm (m) adaptor	Huber+Suhner 32_PC35-50-0-2/199_NE	—	Frequency range: DC to 18 GHz Impedance: 50 Ω Return loss: DC to 1.5 GHz..... ≥ 35 dB 1.5 GHz to 6.0 GHz..... ≥ 30 dB 6.0 GHz to 18.0 GHz..... ≥ 20 dB
3.5 mm (f)-to-3.5 mm (f) adaptor	Huber+Suhner 31_PC35-50-0-2/199_N	—	Frequency range: DC to 18 GHz Impedance: 50 Ω Return loss: DC to 1.5 GHz..... ≥ 35 dB 1.5 GHz to 6.0 GHz..... ≥ 30 dB 6.0 GHz to 18.0 GHz..... ≥ 20 dB
SMA (m)-to-SMA (f) 10 dB attenuator	Huber+Suhner 6610_SMA-50-1/199N	—	Frequency range: DC to 18 GHz Attenuation: 10 dB (nominal) Power rating: 2 W average Impedance: 50 Ω VSWR: DC to 4 GHz..... $\leq 1.15 : 1$ 4 GHz to 8 GHz..... $\leq 1.20 : 1$ 8 GHz to 12.4 GHz..... $\leq 1.25 : 1$ 12.4 GHz to 18 GHz..... $\leq 1.35 : 1$

Table 1. Recommended Equipment for PXIe-5665 Calibration (Continued)

Equipment	Recommended Models	Where Used	Minimum Requirements
SMA (m)-to-SMA (f) 20 dB attenuator	Huber+Suhner 6620_SMA-50-1/199N	—	Frequency range: DC to 18 GHz Attenuation: 20 dB (nominal) Power rating: 2 W average Impedance: 50 Ω VSWR: DC to 4 GHz..... ≤1.15 : 1 4 GHz to 8 GHz..... ≤1.20 : 1 8 GHz to 12. GHz..... ≤1.25 : 1 12.4 GHz to 18 GHz..... ≤1.35 : 1
Power splitter (two-resistor type)	Aeroflex/Weinschel 1593	—	Frequency range: DC to 18 GHz Amplitude tracking: <0.25 dB Phase tracking: <4° Insertion loss: ≤8.5 dB (6 dB, nominal) Power rating: 1 W Impedance: 50 Ω VSWR: DC to 18 GHz..... ≤1.25 : 1 Equivalent output VSWR: DC to 18 GHz..... ≤1.25 : 1 Connectors: 3.5 mm (f)
Anti-distortion test fixture	NI 166375A-01	Verifying third-order intermodulation distortion, Verifying second harmonic intercept, Verifying gain compression	Refer to Appendix A: Anti-Distortion Test Fixture for specifications. Note: The anti-distortion test fixture requires an external +12 VDC supply and USB interface. Contact NI for programming details.

Table 1. Recommended Equipment for PXIe-5665 Calibration (Continued)

Equipment	Recommended Models	Where Used	Minimum Requirements
Frequency reference source	Symmetricom 8040 rubidium frequency standard	—	Frequency: 10 MHz Frequency accuracy: $\pm 1 \times 10^{-9}$
Torque wrench	—	—	Refer to <i>Test Conditions</i> for torque wrench specifications.
* Included in the PXIe-5665 cable accessory kit.			

Test Conditions

The following setup and environmental conditions are required to ensure the PXIe-5665 meets published specifications.

- Keep cabling as short as possible. Long cables and wires act as antennae, picking up extra noise that can affect measurements.
- Verify that all connections, including front panel connections and screws, are secure.
- Maintain an ambient temperature of $23\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$.
- Keep the relative humidity between 10% and 90%, noncondensing.
- Allow a warm-up time of at least 30 minutes after NI-RFSA is loaded and recognizes the PXIe-5665. The warm-up time ensures that the measurement circuitry of the PXIe-5665 is at a stable operating temperature.
- Perform self-calibration on the PXIe-5665.
- Use a torque wrench appropriate for the type of RF connector that you are using. NI recommends a $0.565\text{ N} \cdot \text{m}$ (5 lb · in.) wrench for SMA connectors and a $0.90\text{ N} \cdot \text{m}$ (8 lb · in.) wrench for 3.5 mm connectors.
- Connect the frequency reference source to the REF IN connector on the back of the PXI Express chassis with a standard BNC (m)-to-BNC (m) cable. This connection replaces the connection from the PXIe-5653 REF OUT (10 MHz) connector to the PXI Express chassis REF IN connector, if present.
- Lock all test equipment to the REF OUT signal on the back of the PXI Express chassis. Refer to the *NI 5665 Timing Configurations* topic in the *NI RF Vector Signal Analyzers Help* for more information about configuring clocking sources.
- Ensure that the PXI/PXI Express chassis fan speed is set to HIGH, that the fan filters, if present, are clean, and that the empty slots contain filler panels. For more information, refer to the *Maintain Forced-Air Cooling Note to Users* document available at ni.com/manuals.

System Options

The PXIe-5665 is available with options without certain features. The calibration procedure must be modified to handle the following options:

- No preamplifier: Skip steps in the verification procedures that call for the preamplifier to be enabled.
- 25 MHz instantaneous bandwidth: Verification procedures include any changes necessary to accommodate this option. There are no changes to the PXIe-5665 specifications for this digitizer option.

Initial Setup

Refer to the *NI PXIe-5665 RF Vector Signal Analyzer Getting Started Guide* for information about how to install the software and hardware and how to configure the device in Measurement & Automation Explorer (MAX).

Characterizing the Test System

You use the measured response of the test system during verification tests.

The power splitter and attenuation response is measured at the RF input frequencies used in the verification tests.



Caution The connectors on the device under test (DUT) and test equipment are fragile. Perform the steps in these procedures with great care to prevent damaging any DUTs or test equipment.

Zeroing and Calibrating the Power Sensor

1. Connect channel A of the power meter to power sensor A.
2. Connect channel B of the power meter to power sensor B.
3. Zero and calibrate the power sensors using the built-in functions in the power meter.


Characterizing Power Splitter Reference Output

Designate either of the two outputs of the power splitter as the reference output. This output must be consistently used as the reference output throughout the characterization and verification procedures.

Characterizing Power Splitter Difference

1. Connect the RF source 2 output to the power splitter input through the SMA (m)-to-SMA (m) cable.
2. Connect power sensor A to the reference output of the power splitter through the SMA (m)-to-SMA (m) cable.
3. Connect power sensor B to the other output of the power splitter through the SMA (m)-to-SMA (m) cable. The completed setup is shown in Figure 1.

Figure 1. Power Splitter Difference Characterization Equipment Setup

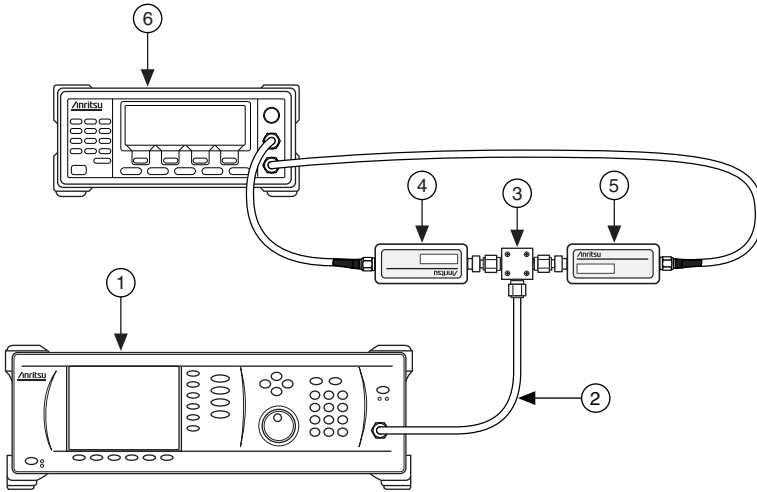

1	RF Source 2	3	Power Splitter	5	Power Sensor B
2	SMA (m)-to-SMA (m) cable	4	Power Sensor A	6	Power Meter

4. Set the RF source 2 frequency to 4 GHz.
5. Set the RF source 2 power to 0 dBm.
6. Measure the signal at 4 GHz with both power sensors.
7. Set the power sensors calibration factor for the measurement frequency at 4 GHz.
8. Calculate the *Power Splitter at 4 GHz Correction Factor* using the following formula:

$$\text{Power Splitter at 4 GHz Correction Factor} = \text{Corrected Power Sensor B Power} - \text{Corrected Power Sensor A Power}$$


Characterizing RF Source Power (Direct)



Note Prior to starting this procedure, zero and calibrate the power sensor according to the [Zeroing and Calibrating the Power Sensor](#) section of this document.

1. Connect the RF source 2 output to the power sensor B input using the SMA (m)-to-SMA (m) cable and 3.5 mm (f)-to-3.5 mm (f) adaptor. The completed equipment setup is shown in Figure 2.

Figure 2. RF Source 2 Output Power Characterization Equipment Setup

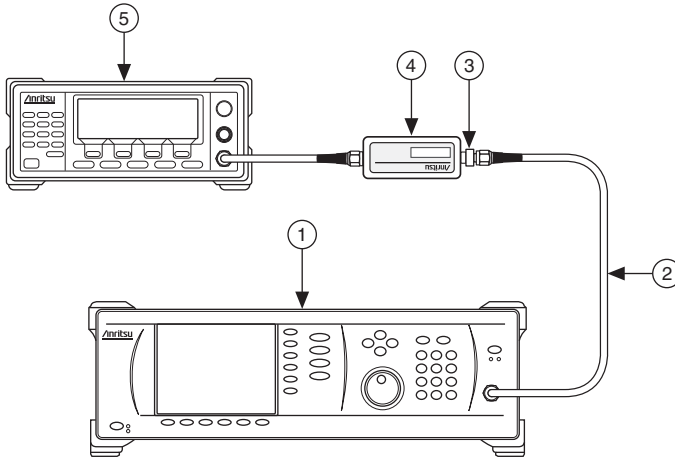

- | | | |
|----------------------------|------------------------------------|---------------|
| 1 RF Source 2 | 3 3.5 mm (f)-to-3.5 mm (f) Adaptor | 5 Power Meter |
| 2 SMA (m)-to-SMA (m) Cable | 4 Power Sensor B | |

2. Set the RF source 2 frequency according to the first row in Table 2 or Table 3 as appropriate.

Table 2. PXIe-5665 3.6 GHz VSA RF Source 2 Characterization Frequencies

Start Frequency	Stop Frequency	Step Size
100.033325 MHz	2.000033325 GHz	100 MHz
2.099966675 GHz	3.599966675 GHz	100 MHz
9.325033325 GHz	11.225033325 GHz	100 MHz
11.324966675 GHz	12.824966675 GHz	100 MHz
1.325033325 GHz	3.225033325 GHz	100 MHz
3.324966675 GHz	4.824966675 GHz	100 MHz
74.966675 MHz	274.966675 MHz	100 MHz

Table 2. PXIe-5665 3.6 GHz VSA RF Source 2 Characterization Frequencies (Continued)

Start Frequency	Stop Frequency	Step Size
25.033325 MHz	1.625033325 GHz	100 MHz
1.724966675 GHz	3.224966675 GHz	100 MHz
3.3875 GHz	—	—
987.5 MHz	—	—

Table 3. PXIe-5665 14GHz VSA RF Source 2 Characterization Frequencies

Start Frequency	Stop Frequency	Step Size
100.033325 MHz	1.975033325 GHz	125 MHz
2.099966675 GHz	3.599966675 GHz	125 MHz
3.724966675 GHz	13.974966675 GHz	125 MHz
13.999966675 GHz	—	—
9.325033325 GHz	11.200033325 GHz	125 MHz
11.324966675 GHz	12.824966675 GHz	125 MHz
4.949966675 GHz	15.199966675 GHz	125 MHz
15.224966675 GHz	—	—
1.325033325 GHz	3.200033325 GHz	125 MHz
3.324966675 GHz	4.824966675 GHz	125 MHz
3.349966675 GHz	13.599966675 GHz	125 MHz
13.624966675 GHz	—	—
24.966675 MHz	274.966675 MHz	125 MHz
1.724966675 GHz	3.224966675 GHz	125 MHz
3.3875 GHz	—	—
987.5 MHz	—	—

- Set the RF source 2 power to 0 dBm.
- Measure the *Channel B Power* using the appropriate calibration factor for the power sensor frequency. Calculate the *RF Source Power Direct* using the following equation:

$$RF\ Source\ Power\ Direct = -Channel\ B\ Power$$

- Repeat steps 2 to 4 for all remaining frequencies in Table 2 or Table 3.


Characterizing RF Source Power (with Lowpass Filter)



Note Prior to starting this procedure, zero and calibrate the power sensor according to the [Zeroing and Calibrating the Power Sensor](#) section of this document.

1. Connect the RF source 2 output to power sensor B through the anti-distortion test fixture. The completed equipment setup is shown in Figure 3.

Figure 3. RF Source Power (with Lowpass Filter) Characterization Equipment Setup

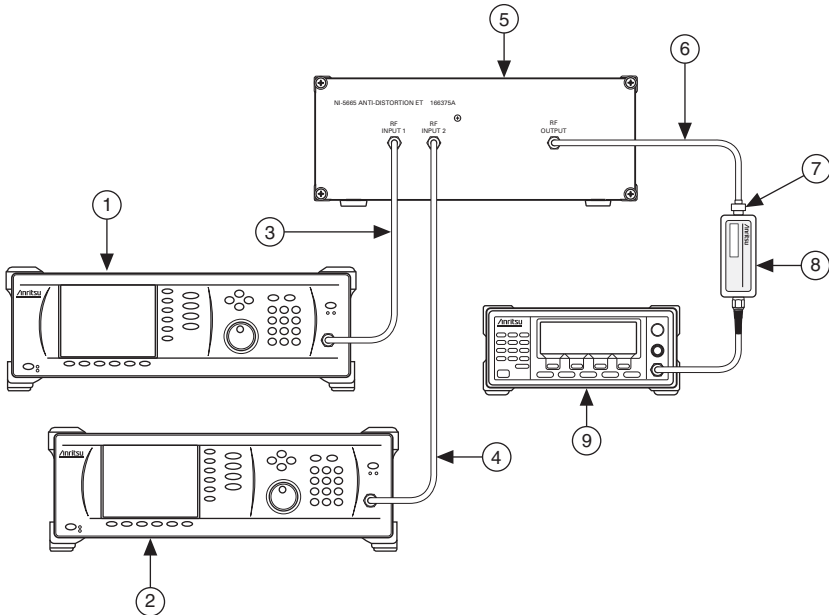

- | | |
|--------------------------------|------------------------------------|
| 1 RF Source 1 | 6 SMA (m)-to-SMA (m) Cable |
| 2 RF Source 2 | 7 3.5 mm (f)-to-3.5 mm (f) Adaptor |
| 3 SMA (m)-to-SMA (m) Cable | 8 Power Sensor B |
| 4 SMA (m)-to-SMA (m) Cable | 9 Power Meter |
| 5 Anti-Distortion Test Fixture | |

2. Disable the RF source 1 output.

- Set the RF source 2 frequency and power according to the first row in Table 4.

Table 4. RF Source 2 Settings

Start Frequency	Stop Frequency	Step Size	Power (dBm)
300 MHz	1.8 GHz	10 MHz	0
1.9 GHz	7.0 GHz	100 MHz	0
300.0333125 MHz	1790.0333125 MHz	10 MHz	-30
1.8 GHz	—	—	-30

- Configure the anti-distortion test fixture to use the appropriate lowpass filter path according to Table 5.

Table 5. Lowpass Filter Frequency Ranges

Lowpass Filter Path (MHz)	Frequency Range
470	1 MHz to 470 MHz
735	>470 MHz to 735 MHz
1,150	>735 MHz to 1.150 GHz
1,800	>1.150 GHz to 1.800 GHz

- Enable the RF source 2 output.
- Measure the channel B power using the appropriate calibration factor for the power sensor frequency. Adjust the RF source 2 power until this measured power is within ± 0.1 dB of the value listed in Table 4. The final RF source 2 power setting is the *RF Source Power LPF* for that frequency.
- Repeat steps 3 to 6 for all the frequencies and powers in Table 4.


Characterizing RF Source Power (Combined) for Frequencies ≤ 700 MHz



Note Prior to starting this procedure, zero and calibrate the power sensor according to the *Zeroing and Calibrating the Power Sensor* section of this document.

1. Connect the RF source 1 and RF source 2 outputs to power sensor B through the anti-distortion test fixture. The completed equipment setup is shown in Figure 4.

Figure 4. RF Source Power (Combined) Characterization Equipment Setup (Frequencies ≤ 700 MHz)

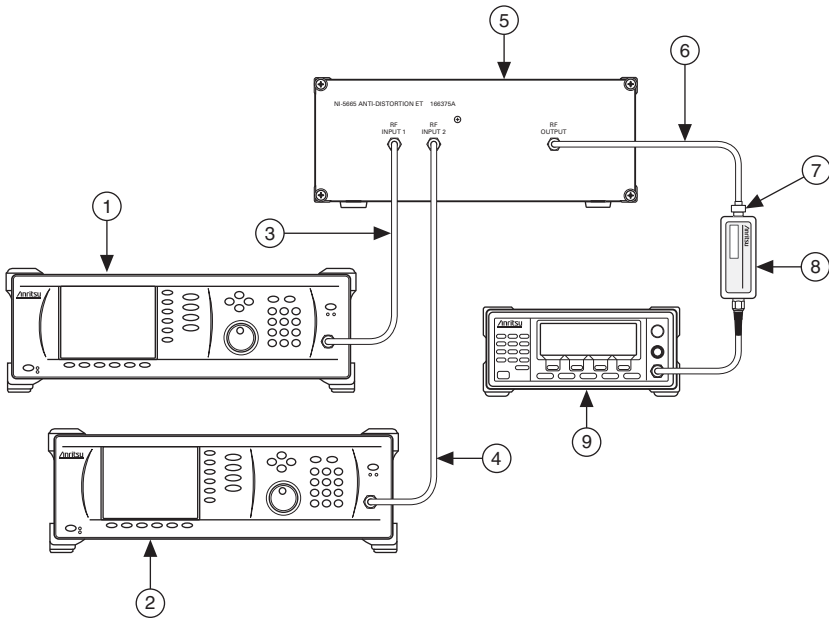

1	RF Source 1	6	SMA (m)-to-SMA (m) Cable
2	RF Source 2	7	3.5 mm (f)-to-3.5 mm (f) Adaptor
3	SMA (m)-to-SMA (m) Cable	8	Power Sensor B
4	SMA (m)-to-SMA (m) Cable	9	Power Meter
5	Anti-Distortion Test Fixture		

2. Set the anti-distortion test fixture to the ≤ 700 MHz combiner path.

- Set the RF source 1 and RF source 2 frequency and power values according to the first row in Table 6.

Table 6. RF Source Power (Combined) Test Settings (Frequencies ≤ 700 MHz)

Start Frequency (MHz)	Stop Frequency (MHz)	Step Size (MHz)	RF Source 1		RF Source 2	
			Frequency Offset	Power (dBm)	Frequency Offset	Power (dBm)
12.05	92.05	10	+350 kHz	-10	-350 kHz	-10
100	700	100	+350 kHz	-10	-350 kHz	-10
12.05	92.05	10	+350 kHz	-30	-350 kHz	-30
100	700	100	+350 kHz	-30	-350 kHz	-30
10	100	10	+1 MHz	+9.1	0 Hz	-24
10	100	10	+1 MHz	-16	0 Hz	-54
200	700	100	+1 MHz	+9.1	0 Hz	-24
200	700	100	+1 MHz	-13	0 Hz	-54
10	100	10	+1 MHz	+8	0 Hz	-24
200	700	100	+1 MHz	+8	0 Hz	-24
10	100	10	+1 MHz	-18	0 Hz	-54
200	700	100	+1 MHz	-15	0 Hz	-54

- Disable the RF source 1 output, and enable the RF source 2 output.



Note When disabled, the RF source 1 output signal should be less than -60 dBm.

- Measure the channel B power using the appropriate sensor calibration factor for the RF source 2 frequency.
- Repeat step 5, adjusting the RF source 2 power until the channel B reading is within ± 0.1 dB of the power listed in Table 6. The RF source 2 power is the *RF Source 2 Programmed Power*.
- Disable the RF source 2 output, and enable the RF source 1 output.



Note When disabled, the RF source 2 output signal should be less than -60 dBm.

- Measure the channel B power using the appropriate sensor calibration factor for the RF source 1 frequency.
- Repeat step 8, adjusting the RF source 1 power until the channel B power is within ± 0.1 dB of the power listed in Table 6. The RF source 1 power is the *RF Source 1 Programmed Power*.
- Repeat steps 3 to 9 for all remaining frequency and power values in Table 6.


Characterizing RF Source Power (Combined) for Frequencies >700 MHz



Note Prior to starting this procedure, zero and calibrate the power sensor according to the [Zeroing and Calibrating the Power Sensor](#) section of this document.

1. Connect the RF source 1 and RF source 2 outputs to power sensor B through the anti-distortion test fixture. The completed equipment setup is shown in Figure 5.

Figure 5. RF Source Power (Combined) Characterization Equipment Setup (Frequencies >700 MHz)

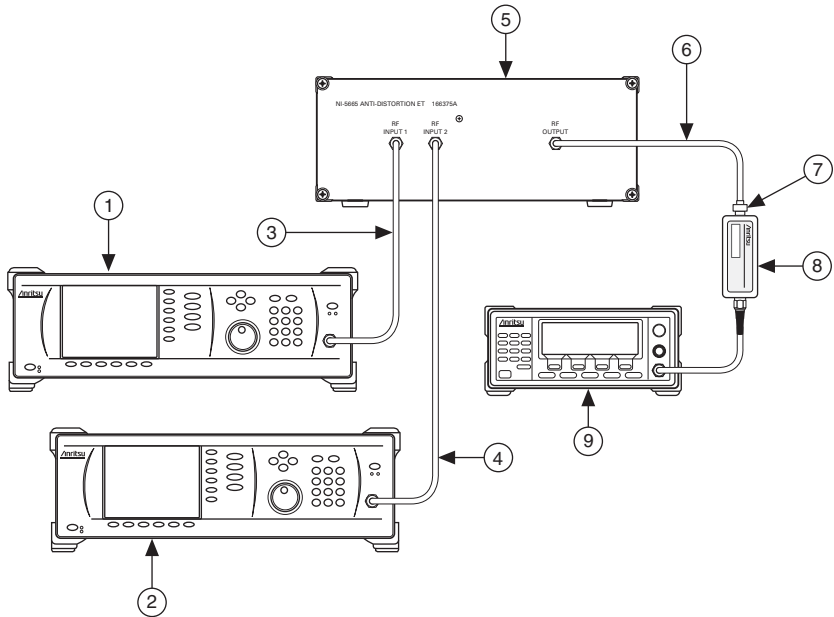

- | | |
|--------------------------------|------------------------------------|
| 1 RF Source 1 | 6 SMA (m)-to-SMA (m) cable |
| 2 RF Source 2 | 7 3.5 mm (f)-to-3.5 mm (f) Adaptor |
| 3 SMA (m)-to-SMA (m) cable | 8 Power Sensor B |
| 4 SMA (m)-to-SMA (m) cable | 9 Power Meter |
| 5 Anti-Distortion Test Fixture | |

2. Set the anti-distortion test fixture to the >700 MHz path.

3. Set the RF source 1 and RF source 2 frequency and power values according to the first row in Table 7.

Table 7. PXIe-5665 RF Source Power (Combined) Test Settings (Frequencies >700 MHz)

Start Frequency	Stop Frequency	Step Size (MHz)	RF Source 1		RF Source 2	
			Frequency Offset	Power (dBm)	Frequency Offset	Power (dBm)
800 MHz	3.500 GHz	100	+350 kHz	-10	-350 kHz	-10
3598.95 MHz	—	—	+350 kHz	-10	-350 kHz	-10
3.6 GHz	13.8 GHz	200	+350 kHz	-10	-350 kHz	-10
13.99895 GHz	—	—	+350 kHz	-10	-350 kHz	-10
800 MHz	3.500 GHz	100	+350 kHz	-30	-350 kHz	-30
3598.95 MHz	—	—	+350 kHz	-30	-350 kHz	-30
3.6 GHz	—	—	+350 kHz	-30	-350 kHz	-30
800 MHz	1.700 GHz	100	+1 MHz	+9.1	0 Hz	-24
800 MHz	1.700 GHz	100	+1 MHz	+8	0 Hz	-24
800 MHz	1.700 GHz	100	+1 MHz	-13	0 Hz	-54
800 MHz	1.700 GHz	100	+1 MHz	-15	0 Hz	-54
1.800 GHz	14.000 GHz	100	+1 MHz	+7.1	0 Hz	-24
1.800 GHz	14.000 GHz	100	+1 MHz	+6	0 Hz	-24
1.800 GHz	3.600 GHz	100	+1 MHz	-16	0 Hz	-54
1.800 GHz	3.600 GHz	100	+1 MHz	-18	0 Hz	-54

4. Disable the RF source 1 output, and enable the RF source 2 output.



Note When disabled, the RF source 1 output signal should be less than -60 dBm.

5. Measure the channel B power using the appropriate sensor calibration factor for the RF source 2 frequency.
6. Repeat step 5, adjusting the RF source 2 power until the channel B reading is within ± 0.1 dB of the power in Table 7. The RF source 2 power is the *RF Source 2 Programmed Power*.
7. Disable the RF source 2 output, and enable the RF source 1 output.



Note When disabled, the RF source 2 output signal should be less than -60 dBm.

8. Measure the channel B power using the appropriate sensor calibration factor for the RF source 1 frequency.
9. Repeat step 8, adjusting the RF source 1 power until the channel B power is within ± 0.1 dB of the power in Table 7. The RF source 1 power is the *RF Source 1 Programmed Power*.
10. Repeat steps 3 to 9 for all remaining frequency and power values listed in Table 7.

Characterizing RF Source Power (Through Splitter)




Note Prior to starting this procedure, zero and calibrate the power sensor and define the power splitter reference output using the procedures in the [Zeroing and Calibrating the Power Sensor](#) and [Characterizing Power Splitter Reference Output](#) sections of this document.

1. Connect the RF source 2 output to the power splitter input through the SMA (m)-to-SMA (m) cable.
2. Connect a 50 Ω termination load to the reference output of the power splitter.

3. Connect power sensor B to the other output of the power splitter through the 3.5 mm (m)-to-3.5 mm (m) adaptors and the 3.5 mm (f)-to-3.5 mm (f) adaptor. The completed equipment setup is shown in Figure 6.

Figure 6. RF Source Power (Through Splitter) Characterization Equipment Setup

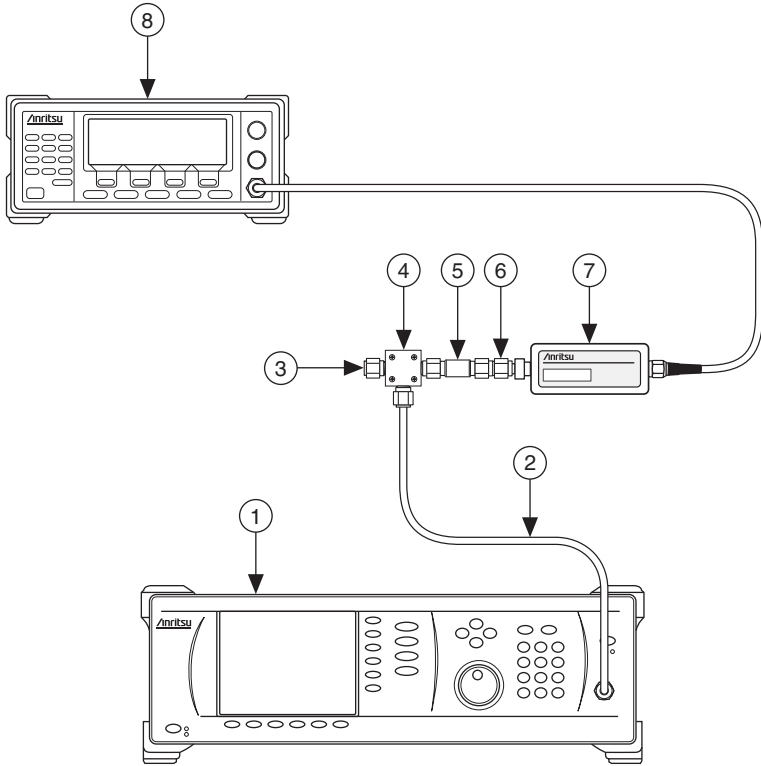

- | | | | |
|---|------------------------------|---|----------------------------------|
| 1 | RF Source 2 | 5 | 3.5 mm (m)-to-3.5 mm (m) Adaptor |
| 2 | SMA (m)-to-SMA (m) Cable | 6 | 3.5 mm (f)-to-3.5 mm (f) Adaptor |
| 3 | 50 Ω Termination Load | 7 | Power Sensor B |
| 4 | Power Splitter | 8 | Power Meter |

4. Set the RF source 2 power to -10 dBm.
5. Set the RF source 2 frequency according to the first row in Table 8.

Table 8. RF Source 2 Frequencies

Start Frequency	Stop Frequency	Step Size
100 MHz	3.5 GHz	200 MHz
3.6 GHz	—	—
3.7 GHz	14 GHz	100 MHz

6. Measure the *Channel B Power* using the appropriate calibration factor for the RF source 2 frequency. Adjust the RF source 2 power until this measured power is within ± 0.1 dB of -10 dBm.
7. Store the RF source 2 set power as the *RF Source Power through Splitter*.
8. Repeat steps 5 to 7 for all remaining frequencies in Table 8.

Characterizing RF Source Power (with Splitter and Attenuator)




Note Prior to starting this procedure, zero and calibrate the power sensor and define the power splitter reference output using the procedures in the [Zeroing and Calibrating the Power Sensor](#) and [Characterizing Power Splitter Reference Output](#) sections of this document.

1. Connect the RF source 2 output to the power splitter input through the SMA (m)-to-SMA (m) cable.
2. Connect power sensor A to the reference output of the power splitter.

3. Connect power sensor B to the other output of the power splitter through the 3.5 mm (m)-to-3.5 mm (m) adaptor, the 3.5 mm (f)-to-3.5 mm (f) adaptor, and the 20 dB attenuator. The completed equipment setup is shown in Figure 7.

Figure 7. RF Source Power (with Splitter and Attenuator) Characterization Equipment Setup

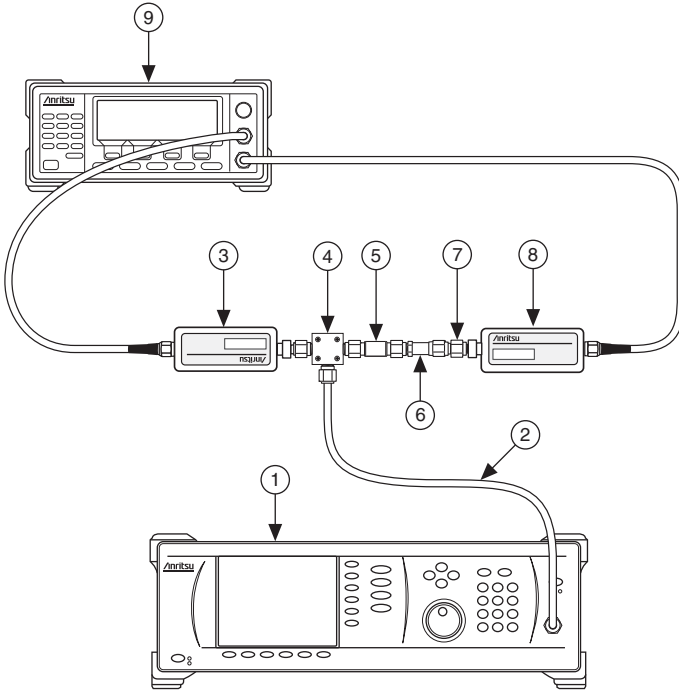

- | | | | |
|---|----------------------------------|---|----------------------------------|
| 1 | RF Source 2 | 6 | 20 dB Attenuator |
| 2 | SMA (m)-to-SMA (m) Cable | 7 | 3.5 mm (f)-to-3.5 mm (f) Adaptor |
| 3 | Power Sensor A | 8 | Power Sensor B |
| 4 | Power Splitter | 9 | Power Meter |
| 5 | 3.5 mm (m)-to-3.5 mm (m) Adaptor | | |

4. Set the RF source 2 power to 0 dBm.

- Set the RF source 2 frequency according to the first row in Table 9.

Table 9. RF Source 2 Frequencies

Start Frequency	Stop Frequency	Step Size
10 MHz	100 MHz	10 MHz
200 MHz	600 MHz	100 MHz
612.5 MHz	—	—
700 MHz	3.6 GHz	100 MHz
3.8 GHz	14 GHz	200 MHz

- Measure the *Channel A Power* and the *Channel B Power* using each sensor and the appropriate calibration factor for the RF source 2 frequency.
- Calculate the *DUT to Power Meter through Attenuator Path Loss* and *RF Source to DUT through Attenuator Path Loss* for that frequency using the following formulas:

$$\text{DUT to Power Meter through Attenuator Path Loss} = \text{Channel A Power} - \text{Channel B Power}$$

$$\text{RF Source to DUT through Attenuator Path Loss} = -\text{Channel B Power}$$


- Repeat steps 5 to 7 for all remaining frequencies in Table 9.

Characterizing Spectrum Analyzer Response

- Connect the RF source 2 output to the power splitter input through the SMA (m)-to-SMA (m) cable.
- Connect power sensor A to the power splitter reference output through the SMA (m)-to-SMA (m) cable.

- Connect the spectrum analyzer to the other power splitter output through the SMA (m)-to-SMA (m) cable. The completed equipment setup is shown in Figure 8.

Figure 8. Spectrum Analyzer Response Characterization Equipment Setup

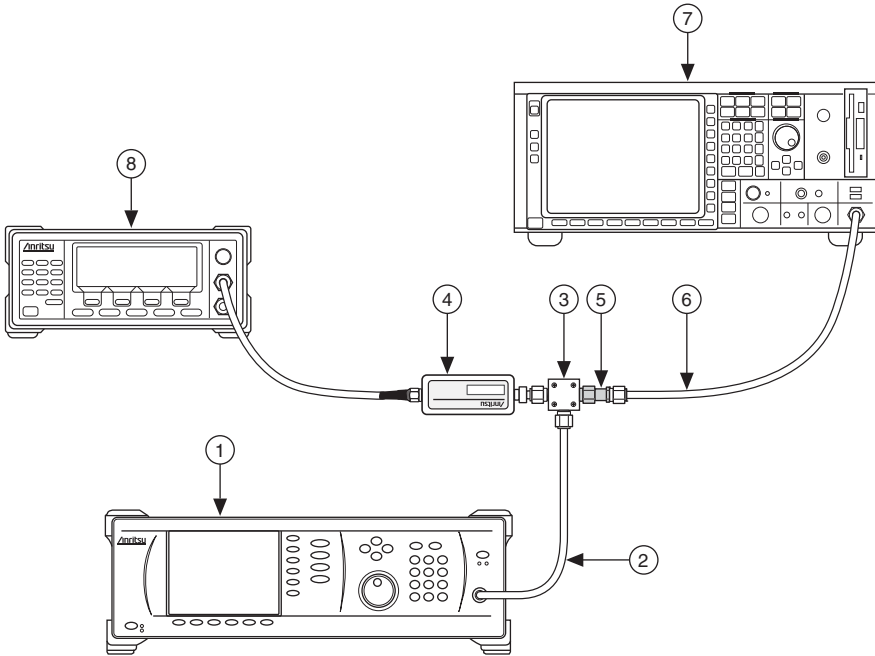

1 RF Source 2	4 Power Sensor A	7 Spectrum Analyzer
2 SMA (m)-to-SMA (m) cable	5 10 dB Attenuator	8 Power Meter
3 Power Splitter	6 SMA (m)-to-SMA (m) cable	

- Set the RF source 2 power to 0 dBm.
- Set the RF source 2 frequency to 4 GHz.
- Configure the spectrum analyzer according to the following settings:
 - Resolution bandwidth: 1 kHz
 - Center frequency: 4 GHz
 - Frequency span: 0 Hz
 - Reference level: 0 dBm
- Measure the power sensor A power.
- Correct the power sensor A measured power for the measurement frequency of 4 GHz.
- Correct the power sensor A measured power for the *Power Splitter at 4 GHz Correction Factor* from the *Characterizing Power Splitter Difference* equipment characterization section of this document using the following equation:

$$\text{Corrected Power Sensor Power} = \text{Power Sensor A reading} + \text{Power Splitter at 4 GHz Correction Factor}$$

10. Measure the spectrum analyzer peak power.
11. Calculate the *Spectrum Analyzer Correction Factor* using the following formula:

$$\text{Spectrum Analyzer Correction Factor} = \frac{\text{Corrected Power Sensor Power}}{\text{Spectrum Analyzer Power}}$$

As-Found and As-Left Limits

The as-found limits are the published specifications for the PXIe-5665. NI uses these limits to determine whether the PXIe-5665 meets the device specifications when it is received for calibration.

The as-left limits are equal to the published NI specifications for the PXIe-5665, less guard bands for manufacturing test measurement uncertainty, temperature drift, and drift over time. NI uses these limits to determine whether the PXIe-5665 meets the device specifications over its calibration interval.

Verification

The performance verification procedures assume that adequate traceable uncertainties are available for the calibration references.

In the event of a failure during the verification of the PXIe-5665, perform a calibration of the individual modules. Return the PXIe-5603 or PXIe-5605 module to NI for calibration and adjustment, if needed.


Verifying Reference Accuracy

The PXIe-5665 reference accuracy specification is derived from the PXIe-5653 reference accuracy. For more information about PXIe-5653 calibration values, refer to the *NI PXIe-5653 Calibration Procedure* available at ni.com/manuals.

Verifying Phase Noise

The phase noise for the PXIe-5665 system is determined by the phase noise of the PXIe-5653 module. To verify the PXIe-5653 phase noise specification, you must use the phase noise verification test for the PXIe-5653. For more information about calibration and verification of the PXIe-5653, refer to the *NI PXIe-5653 Calibration Procedure*, available at ni.com/manuals.

Figure 10. PXIe-5665 14 GHz VSA Frequency Response and Absolute Amplitude Accuracy Verification (Frequencies >10 MHz) Equipment Setup

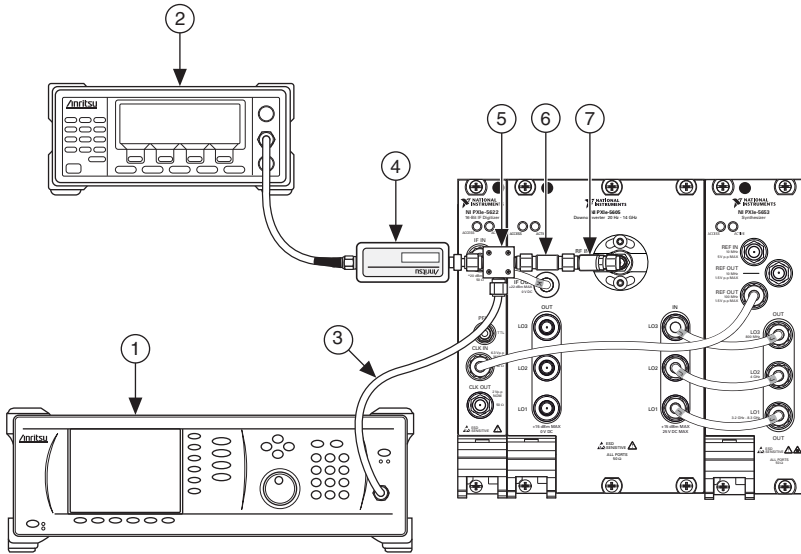

- | | |
|----------------------------|------------------------------------|
| 1 RF Source 2 | 5 Power Splitter |
| 2 Power Meter | 6 3.5 mm (m)-to-3.5 mm (m) Adaptor |
| 3 SMA (m)-to-SMA (m) cable | 7 20 dB Attenuator |
| 4 Power Sensor A | |

4. Create a new session for the PXIe-5665.
5. Configure the PXIe-5665 according to the following fixed property settings. These settings remain unchanged during the test.
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 10
 - Digital IF Equalization Enabled: TRUE
 - Digitizer Dither Enabled: Enabled
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - Span: 100 kHz
 - Resolution Bandwidth: 10 kHz
6. Configure the PXIe-5665 according to the following variable property settings:
 - Preamp Enabled: Disabled
 - Device Instantaneous Bandwidth: 300 kHz
 - **(PXIe-5665 14 GHz VSA)** Preselector Enabled: Disabled

7. Set the PXIe-5665 reference level using the following values:
 - Start power: -50 dBm
 - Stop power: -10 dBm
8. Set the PXIe-5665 center frequency and the RF source 2 frequency according to the first row in Table 10.

Table 10. Frequency Response and Absolute Amplitude Accuracy Verification (Frequencies >10 MHz) Test Frequencies

Start Frequency	Stop Frequency	Step Size
10 MHz*	100 MHz	30 MHz
200 MHz	600 MHz	200 MHz
612.5 MHz	—	—
800 MHz	3.6 GHz	400 MHz
4 GHz	14 GHz	500 MHz

* The 10 MHz to 100 MHz frequency range applied only to the 300 kHz device instantaneous bandwidth value.

9. Set the RF source 2 amplitude for that RF source 2 frequency using the following equation:

$$RF\ Source\ 2\ Amplitude = PXIe-5665\ Reference\ Level + \\ RF\ Source\ to\ DUT\ through\ Attenuator\ Path\ Loss$$

10. Commit the PXIe-5665 settings to hardware.
11. Take five readings of the RF source 2 amplitude using power sensor A. Calculate the average power.
12. Repeat step 11 until any two readings measured differ no more than 0.02 dB and no two averages differ by more than 0.005 dB. This average is the *Measured Average Power*.



Note More than 30 averages total indicate a test failure that you must diagnose.

13. Calculate the *Corrected Input Power* using the following formula:

$$Corrected\ Input\ Power = Measured\ Average\ Power - \\ DUT\ to\ Power\ Meter\ through\ Attenuator\ Path\ Loss$$



Note The *RF Source to DUT through Attenuator Path* and *DUT to Power Meter through Attenuator Path Loss* values were measured in the [Characterizing RF Source Power \(with Splitter and Attenuator\)](#) equipment characterization procedure. Use the values that correspond to the frequency range you are testing.

14. Read the PXIe-5665 power spectrum. The *PXIe-5665 Power* is the peak value of that spectrum.

15. Calculate the *Absolute Amplitude Accuracy* at each RF frequency using the following formula:

$$\text{Absolute Amplitude Accuracy} = \text{PXIe-5665 Power} - \text{Corrected Input Power}$$

16. Repeat steps 8 to 15 for all remaining frequencies in Table 10.
17. Calculate the *Frequency Response* at each RF frequency using the following formula:

$$\text{Frequency Response} = \text{Absolute Amplitude Accuracy} - \text{Absolute Amplitude Accuracy at 612.5 MHz}$$



Note Calculate *Frequency Response* only for PXIe-5665 center frequencies less than or equal to 3.6 GHz.

18. Repeat steps 9 to 17 for all reference levels listed in step 7.
19. Repeat steps 8 to 18 for an instantaneous bandwidth of 50 MHz (25 MHz for the PXIe-5665 with 25 MHz bandwidth).
20. Repeat steps 8 to 19 with the PXIe-5665 preamplifier enabled.
21. **(PXIe-5665 14 GHz VSA)** Repeat steps 8 to 19 for test frequencies greater than 3.6 GHz with the PXIe-5665 preselector enabled and preamplifier disabled.



Note The PXIe-5665 preselector has a maximum instantaneous bandwidth of 47 MHz. For steps that call for a 50 MHz instantaneous bandwidth, use a 40 MHz instantaneous bandwidth when using the preselector.

22. Compare the *Frequency Response* to the verification test limits in Table 11 or Table 12 as appropriate.

Table 11. Frequency Response Verification Test Limits (Preamplifier Disabled)

Frequency	Device	As-Found Limit (dB)	As-Left Limit (dB)*
10 MHz to 100 MHz	PXIe-5665	±0.60	±0.35
>100 MHz to 1.7 GHz		±0.35	±0.25
>1.7 GHz to 2.8 GHz	PXIe-5665 3.6 GHz VSA	±0.40	±0.30
	PXIe-5665 14 GHz VSA	±0.42	
>2.8 GHz to 3.6 GHz	PXIe-5665 3.6 GHz VSA	±0.45	±0.35
	PXIe-5665 14 GHz VSA	±0.62	

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

Table 12. Frequency Response Verification Test Limits (Preamplifier Enabled)

Frequency	Device	As-Found Limit (dB)	As-Left Limit (dB)*
10 MHz to 100 MHz	PXIe-5665	±0.75	±0.50
>100 MHz to 2.8 GHz		±0.45	±0.30
>2.8 GHz to 3.6 GHz	PXIe-5665 3.6 GHz VSA	±0.45	±0.30
	PXIe-5665 14 GHz VSA	±0.50	±0.45

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

23. Compare the *Absolute Amplitude Accuracy* to the verification test limits in Table 13, Table 14, or Table 15 as appropriate.

Table 13. Absolute Amplitude Accuracy Verification Test Limits
(Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Disabled)

Frequency	Device	As-Found Limit (dB)	As-Left Limit (dB)*
612.5 MHz	PXIe-5665 3.6 GHz VSA	±0.35	±0.25
	PXIe-5665 14 GHz VSA	±0.46	±0.38
10 MHz to 100 MHz	PXIe-5665 3.6 GHz VSA	±0.95	±0.60
	PXIe-5665 14 GHz VSA	±1.06	±0.73
>100 MHz to 1.7 GHz	PXIe-5665 3.6 GHz VSA	±0.70	±0.50
	PXIe-5665 14 GHz VSA	±0.81	±0.63
>1.7 GHz to 2.8 GHz	PXIe-5665 3.6 GHz VSA	±0.75	±0.55
	PXIe-5665 14 GHz VSA	±0.88	±0.68
>2.8 GHz to 3.6 GHz	PXIe-5665 3.6 GHz VSA	±0.80	±0.60
	PXIe-5665 14 GHz VSA	±1.08	±0.73
>3.6 GHz to 7.5 GHz	PXIe-5665 14 GHz VSA	±0.70	±0.50
>7.5 GHz to 8.5 GHz		±0.80	±0.50
>8.5 GHz to 14 GHz		±1.25	±0.75

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

Table 14. Absolute Amplitude Accuracy Verification Test Limits (Preamplifier Enabled)

Frequency	Device	As-Found Limit (dB)	As-Left Limit (dB)*
612.5 MHz	PXIe-5665 3.6 GHz VSA	±0.35	±0.30
	PXIe-5665 14 GHz VSA	±0.70	±0.60
10 MHz to 100 MHz	PXIe-5665 3.6 GHz VSA	±1.10	±0.80
	PXIe-5665 14 GHz VSA	±1.45	
>100 MHz to 2.8 GHz	PXIe-5665 3.6 GHz VSA	±0.80	±0.60
	PXIe-5665 14 GHz VSA	±1.15	
>2.8 GHz to 3.6 GHz	PXIe-5665 3.6 GHz VSA	±0.80	±0.60
	PXIe-5665 14 GHz VSA	±1.20	±0.75

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

Table 15. PXIe-5665 14 GHz VSA Absolute Amplitude Accuracy Verification Test Limits (Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Enabled)

Frequency	As-Found Limit (dB)	As-Left Limit (dB)*
>3.6 GHz to 7.5 GHz	±4.0	±1.5
>7.5 GHz to 8.5 GHz	±4.0	±1.5
>8.5 GHz to 14 GHz	±4.0	±1.5

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.


24. Close the PXIe-5665 session.

If the frequency response and absolute amplitude accuracy verification procedures determines that the PXIe-5665 is outside its limits, refer to *Worldwide Support and Services* for information about support resources or service requests.

Verifying Average Noise Level


1. Connect a 50 Ω termination to the PXIe-5665 RF IN connector. The completed equipment setup is shown in Figure 11 and Figure 12.

Figure 11. PXIe-5665 3.6 GHz VSA Average Noise Level Verification Equipment Setup

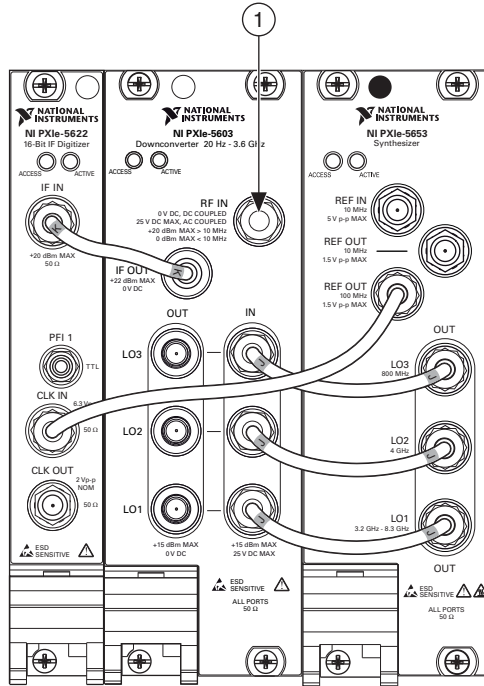

1 50 Ω termination

Figure 12. PXIe-5665 14 GHz VSA Average Noise Level Verification Equipment Setup

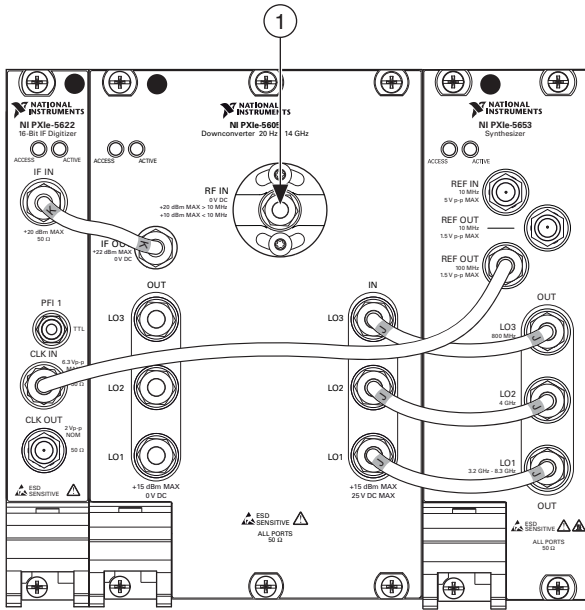

1 50 Ω termination

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averages
 - Channel Coupling: AC Coupled
 - Digital IF Equalization Enabled: TRUE
 - Digitizer Dither Enabled: Enabled
 - Number of Averages: 20
 - Ref Clock Source: PXI_Clk
 - Power Spectrum Units: Volts Squared
 - Preamp Enabled: Disabled
 - Resolution Bandwidth Type: ENBW
 - Reference Level: -50 dBm
 - Resolution Bandwidth: 300 Hz
 - RF Attenuation: 0 dB
 - FFT Window Type: Blackman-Harris
 - **(PXIe-5665 14 GHz VSA) Preselector Enabled: Disabled**

- Set the PXIe-5665 center frequency according to Table 16.

Table 16. Average Noise Level Verification Test Frequencies

Start Frequency	Stop Frequency	Step Size (MHz)
10 MHz	90 MHz	20
100 MHz	3.6 GHz	500
4 GHz	14 GHz	500

- Set the PXIe-5665 channel coupling, RF attenuation, device instantaneous bandwidth, span, resolution bandwidth, sampling ratio, and number of averages according to Table 17.

Table 17. PXIe-5665 Settings for Average Noise Level Verification

Test Frequency	Device Instantaneous Bandwidth	Span	OSP Sampling Ratio
10 MHz to <100 MHz	300 kHz	100 kHz	32
100 MHz to \leq 3.6 GHz	300 kHz	100 kHz	32
	50 MHz*	5 MHz	1
3.8 GHz to 14 GHz	50 MHz*	5 MHz	1

* Set the PXIe-5665 Device Instantaneous Bandwidth to 25 MHz for the PXIe-5665 with 25 MHz bandwidth.

- Commit the PXIe-5665 settings to hardware.
- Read the power spectrum from the PXIe-5665. Convert the power spectrum to a power spectral density (dBm/Hz) value.
- Remove five points from around the center of the power spectral density from step 7.
- Convert the power spectral density with the points removed to watts/Hz, take the mean, and then convert the result back to dBm/Hz. This value is the *PXIe-5665 Average Noise (dBm/Hz)*.
- Repeat steps 4 to 9 for all frequencies in Table 16.
- Repeat steps 4 to 10 for frequencies less than or equal to 3.6 GHz with the PXIe-5665 preamplifier enabled.
- (PXIe-5665 14 GHz VSA)** Repeat steps 4 to 10 for frequencies greater than 3.6 GHz with the PXIe-5665 preselector enabled and preamplifier disabled.



Note The PXIe-5665 preselector has a maximum instantaneous bandwidth of 47 MHz. For steps that call for a 50 MHz instantaneous bandwidth, use a 40 MHz instantaneous bandwidth when using the preselector.

13. Compare the *PXIe-5665 Average Noise (dBm/Hz)* to the verification test limits in Table 18, Table 19, or Table 20 as appropriate.

Table 18. Average Noise Verification Test Limits (Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Disabled)

Frequency	As-Found Limit (dBm/Hz)	As-Left Limit* (dBm/Hz)
>10 MHz to 100 MHz	-149	-151
>100 MHz to 300 MHz	-152	-154
>300 MHz to 1.7 GHz	-151	-153
>1.7 GHz to 2.8 GHz	-149	-151
>2.8 GHz to 3.6 GHz	-148	-150
>3.6 GHz to 7.5 GHz [†]	-148	-150
>7.5 GHz to 8.5 GHz [†]	-146	-147
>8.5 GHz to 12 GHz [†]	-147	-148
>12 GHz to 14 GHz [†]	-145	-146

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

[†] Frequencies >3.6 GHz apply only to the PXIe-5665 14 GHz VSA.

Table 19. Average Noise Verification Test Limits (Preamplifier Enabled)

Frequency	As-Found Limit (dBm/Hz)	As-Left Limit* (dBm/Hz)
>10 MHz to 100 MHz	-161	-163
>100 MHz to 300 MHz	-162	-165
>300 MHz to 1.7 GHz	-162	-164
>1.7 GHz to 2.8 GHz	-161	-163
>2.8 GHz to 3.6 GHz	-160	-163

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

Table 20. Average Noise Verification Test Limits (Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Enabled)

Frequency	As-Found Limit (dBm/Hz)	As-Left Limit* (dBm/Hz)
>3.6 GHz to 7.5 GHz	-144	-145
>7.5 GHz to 8.5 GHz	-140	-141
>8.5 GHz to 12 GHz	-141	-142
>12 GHz to 14 GHz	-140	-141
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.		


14. Close the PXIe-5665 session.

If the average noise level verification procedure determines that the PXIe-5665 is outside its limits, refer to *Worldwide Support and Services* for information about support resources or service requests.

Verifying Non-Input-Related Spurs (Residual Spurs)


1. Connect a 50 Ω termination to the PXIe-5665 RF IN connector. The completed equipment setup is shown in Figure 13 and Figure 14.

Figure 13. PXIe-5665 3.6 GHz VSA Non-Input-Related Spurs Verification Equipment Setup

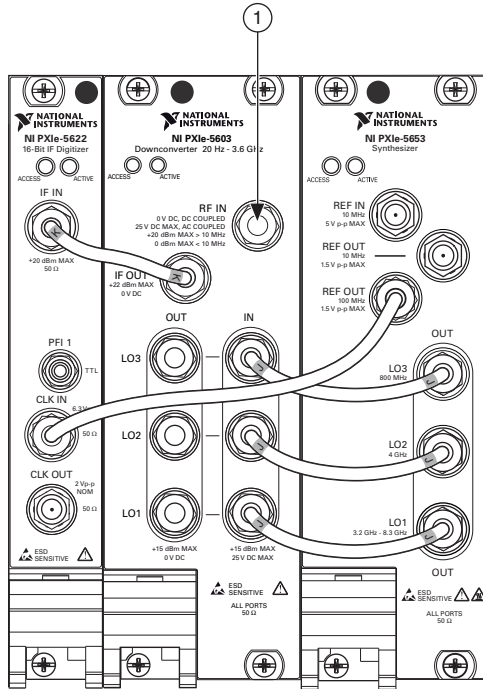

1 50 Ω Termination

Figure 14. PXIe-5665 14 GHz VSA Non-Input-Related Spurs Verification Equipment Setup

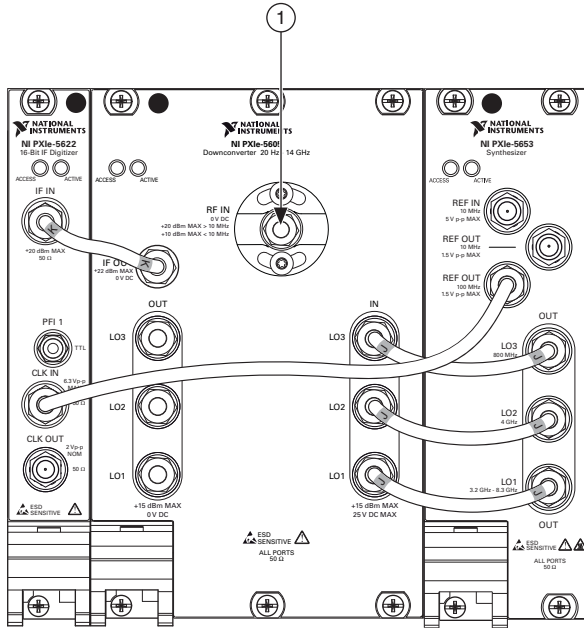

1 50 Ω Termination

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 4
 - Ref Clock Source: PXI_Clk
 - Ref Clock Rate: 10 MHz
 - Channel Coupling: AC Coupled
 - Preamp Enabled: Disabled
 - Span: 50 MHz (25 MHz for the PXIe-5665 with 25 MHz bandwidth)
 - Device Instantaneous Bandwidth: 50 MHz (25 MHz for the PXIe-5665 with 25 MHz bandwidth)
 - Resolution Bandwidth: 2 kHz
 - RF Attenuation: 0 dB
 - Reference Level: -60 dBm
 - FFT Window Type: Flat Top
 - **(PXIe-5665 14 GHz VSA)** Preselector Enabled: Disabled

4. Set the PXIe-5665 center frequency using the following values:
 - Start frequency: 100 MHz
 - Stop frequency:
 - **(PXIe-5665 3.6 GHz VSA)** 3.6 GHz
 - **(PXIe-5665 14 GHz VSA)** 14 GHz
 - Step size: 9.997331 MHz
5. Commit the PXIe-5665 settings to hardware.
6. Read the power spectrum from the PXIe-5665.
7. Measure the highest power in the spectrum returned from the PXIe-5665. This value is the *PXIe-5665 Non-Input-Related Spurious Level*.
8. Repeat steps 4 to 7 for all frequencies in step 4.
9. Compare the *PXIe-5665 Non-Input-Related Spurious Level* to the verification test limits in Table 21.

Table 21. Non-Input-Related Spurs Verification Test Limits

Center Frequency	As-Found Limit (dBm)	As-Left Limit (dBm)*
100 MHz to <1.650 GHz	-95	-96
1.650 GHz to 1.750 GHz	-85	-88
>1.750 GHz to 3.6 GHz	-95	-96
>3.6 GHz to 7.5 GHz†	-92	-94
>7.5 GHz to 8.5 GHz†	-90	-92
>8.5 GHz to 14 GHz†	-90	-92
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.		
† Center frequencies >3.6 GHz apply only to the PXIe-5665 14 GHz VSA.		


10. Close the PXIe-5665 session.

If the non-input-related spurs (residual spurs) verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

Verifying LO-Related Spurs (Sideband Spurs)


1. Connect RF source 2 to the power splitter input through the SMA (m)-to-SMA (m) cable.
2. Connect the power splitter reference output to the spectrum analyzer through the SMA (m)-to-SMA (m) cable.
3. Connect the other power splitter output to the PXIe-5665 RF IN connector using the 3.5 mm (m)-to-3.5 mm (m) adaptor. The completed equipment setup is shown in Figure 15 and Figure 16.

Figure 15. PXIe-5665 3.6 GHz VSA LO-Related Spurs Verification Equipment Setup

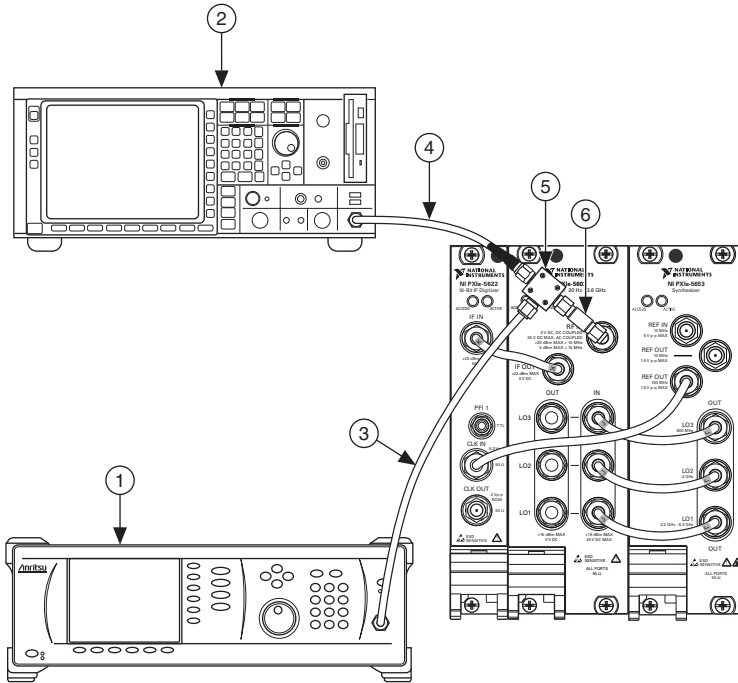

- | | | | |
|---|--------------------------|---|----------------------------------|
| 1 | RF Source 2 | 4 | SMA (m)-to-SMA (m) cable |
| 2 | Spectrum Analyzer | 5 | Power Splitter |
| 3 | SMA (m)-to-SMA (m) cable | 6 | 3.5 mm (m)-to-3.5 mm (m) Adaptor |

Figure 16. PXIe-5665 14 GHz VSA LO-Related Spurs Verification Equipment Setup

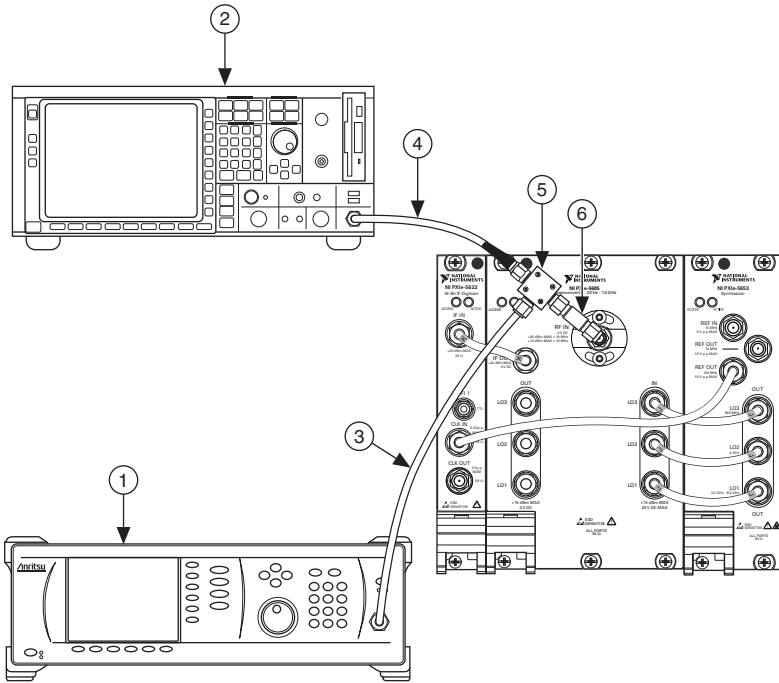

- | | |
|----------------------------|------------------------------------|
| 1 RF Source 2 | 4 SMA (m)-to-SMA (m) cable |
| 2 Spectrum Analyzer | 5 Power Splitter |
| 3 SMA (m)-to-SMA (m) cable | 6 3.5 mm (m)-to-3.5 mm (m) Adaptor |

4. Create a new session for the PXIe-5665.

5. Configure the PXIe-5665 according to the following fixed property settings. These settings remain unchanged during the test.
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 10
 - Ref Clock Source: PXI_Clk
 - Ref Clock Rate: 10 MHz
 - Preamp Enabled: Disabled
 - Reference Level: -10 dBm
 - FFT Window Type: Flat Top
 - Resolution Bandwidth Type: Bin Width
 - Channel Coupling: AC Coupled
 - Device Instantaneous Bandwidth: 50 MHz (25 MHz for the PXIe-5665 with the 25 MHz bandwidth)
 - **(PXIe-5665 14 GHz VSA)** Preselector Enabled: Disabled
6. Set the RF source 2 mode to Single Frequency.
7. Connect the frequency reference source to the spectrum analyzer reference frequency input.
8. Set the spectrum analyzer reference source to External.



Note If the RF source you use for this test has consistent, known offset spurs, these spurs can be characterized independently of the LO-related spurs. You can ignore these offset frequencies to save time during testing.

9. Set the PXIe-5665 center frequency according to the first row in either Table 22 or Table 23.

Table 22. PXIe-5665 3.6 GHz VSA Test Frequencies

Start Frequency	Stop Frequency	Step Size
100 MHz	3.5 GHz	200 MHz
3.6 GHz	—	—

Table 23. PXIe-5665 14 GHz VSA Test Frequencies

Start Frequency	Stop Frequency	Step Size
100 MHz	13.9 GHz	200 MHz
14 GHz	—	—

10. Configure the RF Source 2 according to the following settings:
 - Center frequency: PXIe-5665 center frequency
 - Output power: *RF Source Power through Splitter* for that frequency
11. Set the spectrum analyzer center frequency to the RF source 2 frequency.
12. Set the PXIe-5665 span and resolution bandwidth according to the first row in Table 24.

Table 24. LO-Related Spurs Verification Bandwidth and Span Settings

PXIe-5665 Span	PXIe-5665 RBW	PXIe-5665 Notch BW (Number of Bins at Stated RBW)	Spectrum Analyzer Span	Spectrum Analyzer RBW	Spectrum Analyzer Averages
200 kHz	10 Hz	20 kHz (1999)	600 Hz	50 Hz	6
2 MHz	40 Hz	200 kHz (4999)	300 Hz	50 Hz	3
20 MHz	60 Hz	2 MHz (33333)	300 Hz	50 Hz	3

13. Set the spectrum analyzer span, resolution bandwidth, and number of averages according to the values in Table 24.
14. Commit the PXIe-5665 settings to hardware.
15. Wait 250 ms before making the first measurement and wait 100 ms before making a subsequent measurements to allow the PXIe-5665 and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the [Test Equipment](#) section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

16. Measure the RF source 2 spectrum with the spectrum analyzer.
17. Perform a peak search on the spectrum from step 16. The value of the peak is the *Spectrum Analyzer Tone Power*. This value is used in step 19(c).

18. Measure the spectrum on the PXIe-5665.
 - a. Find the peak value of the spectrum.
 - b. Confirm that the peak value is between -16 dBm and -4 dBm. The peak value is the *PXIe-5665 Tone Power*. This value is used in step 18(d).
 - c. Notch filter the spectrum by replacing the appropriate number of bins from the center of the spectrum according to Table 24 with bins of -130 dB in value. The resulting spectrum is the *Notched Spectrum*.
 - d. Calculate the *Notched Spectrum Response* using the following equation:

$$\text{Notched Spectrum Response (dB)} = \text{Notched Spectrum (dBm)} - \text{PXIe-5665 Tone Power (dBm)}$$

- e. Create a list of target spurs from the *Notched Spectrum Response* (dB) that have a level greater than -90 dB.
- f. If any two spurs are within ± 500 Hz of each other, retain only the spur with the greater power magnitude. This reduced list is used in step 19(a).



Note The RF source 2 indicated for use in this procedure exhibits spurious responses that have a frequency spread of 500 Hz. Any target spur found within ± 500 Hz of an RF source 2 spurious response is considered to be from the RF source 2 because of this frequency spread.

19. Eliminate any RF source 2 spurious responses from the list of target spurs.
 - a. Tune the spectrum analyzer to the frequency of each target spur in the reduced list from step 18(f).
 - b. Measure the spectrum and perform a peak search on the measured spectrum. This value is the *Spectrum Analyzer Peak Value*.
 - c. Convert the *Spectrum Analyzer Peak Value* units to dB using the following equation:

$$\text{Spectrum Analyzer Peak (dB)} = \text{Spectrum Analyzer Peak Value (dBm)} - \text{Spectrum Analyzer Tone Power}$$
 - d. If the value of the *Spectrum Analyzer Peak (dB)* is 5 dB or more below the spur level in the reduced list from step 18(f), retain the spur level, otherwise discard the value.
20. Compare the spur values from the sorted list in step 19(d) to the verification test limits in Table 25.

Table 25. LO-Related Spurious Responses (Sideband Spurs)
Verification Test Limits

Center Frequency	As-Found Limit (dBc)	As-Left Limit (dBc) [*]
100 MHz to 3.6 GHz	-73	-75
3.6 GHz to 14 GHz [†]	-73	-75
[*] Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits. [†] Center frequencies >3.6 GHz apply only to the PXIe-5665 14 GHz VSA.		

21. Repeat steps 11 to 19 for all spans in Table 24.
22. Repeat steps 9 to 20 for all center frequencies in Table 22.
23. **(PXIe-5665 14 GHz VSA)** Repeat steps 9 to 20 for center frequencies from 3.8 GHz to 14 GHz in 200 MHz steps with the PXIe-5665 preselector enabled.



Note The PXIe-5665 preselector has a maximum instantaneous bandwidth of 47 MHz. For steps that call for a 50 MHz instantaneous bandwidth, use a 40 MHz instantaneous bandwidth when using the preselector.

24. Close the PXIe-5665 session.

If the LO-related spurs (sideband spurs) verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

Verifying Image Rejection

This procedure verifies the following image responses of the PXIe-5665:

For test frequencies <3.6 GHz:

- $IF1 \text{ Image} = \text{Test Frequency} + 9.225 \text{ GHz}$
- $IF2 \text{ Image} = 3.3875 \text{ GHz}$
- $IF3 \text{ Image} = 987.5 \text{ MHz}$
- $IF2 \text{ Image at RF} = \text{Test Frequency} + 1.225 \text{ GHz}$
- $IF3 \text{ Image at RF} = |\text{Test Frequency} - 375 \text{ MHz}|$ (Evaluated only for images greater than 10 MHz)


For test frequencies >3.6 GHz,

- $IF1 \text{ Image} = \text{Test Frequency} + 1.225 \text{ GHz}$
- $IF2 \text{ Image} = 987.5 \text{ GHz}$
- $IF2 \text{ Image at RF} = \text{Test Frequency} - 375 \text{ MHz}$

where *Test Frequency* is the PXIe-5665 center frequency.

1. Connect RF source 2 to the PXIe-5665 RF IN using the SMA (m)-to-SMA (m) cable. The completed equipment setup is shown in Figure 17 and Figure 18.


Figure 17. PXIe-5665 3.6 GHz VSA Image Rejection Verification Equipment Setup

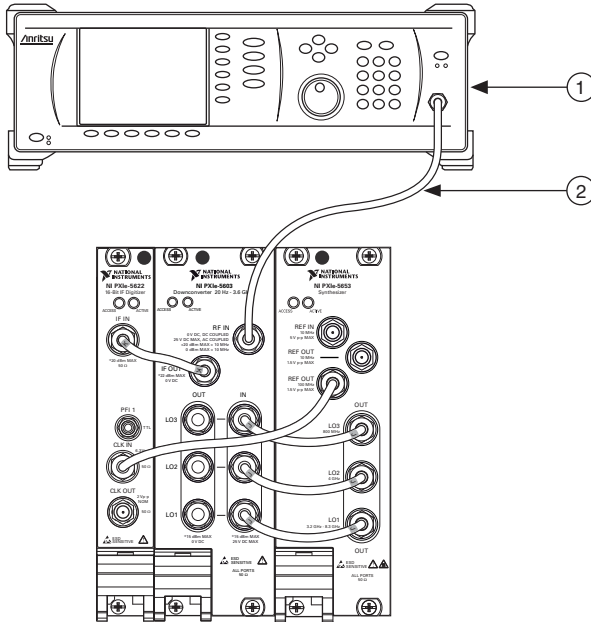

1 RF Source 2

2 SMA (m)-to-SMA (m) cable

Figure 18. PXIe-5665 14 GHz VSA Image Rejection Verification Equipment Setup

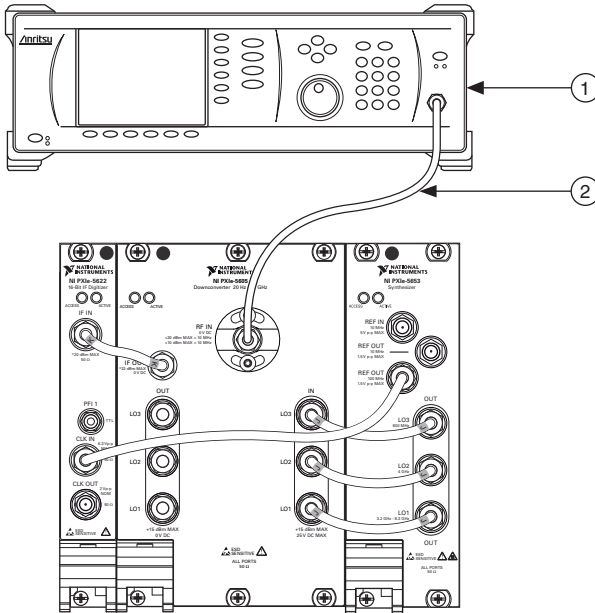

1 RF Source 2

2 SMA (m)-to-SMA (m) cable

2. Create a new session for the PXIe-5665.
3. Configure the RF source 2 using the following values:
 - Mode: Single frequency
 - Power level: 0 dBm
4. Configure the PXIe-5665 according to following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 20
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - Preamp Enabled: Disabled
 - Span: 20 kHz
 - Resolution Bandwidth: 100 Hz
 - Device Instantaneous Bandwidth: 40 MHz (25 MHz for the PXIe-5665 with 25 MHz bandwidth)
 - RF Attenuation: 10 dB
 - Reference Level: 0 dBm
 - **(PXIe-5665 14 GHz VSA) Preselector Enabled: Enabled**

- Set the PXIe-5665 center frequency according to Table 26 or Table 27 as appropriate.

Table 26. PXIe-5665 3.6 GHz VSA Image Rejection Verification Test Frequencies

Start Frequency	Stop Frequency (GHz)	Step Size (MHz)
100.033325 MHz	2.000033325	400
2.399966675 GHz	3.599966675	400

Table 27. PXIe-5665 14 GHz VSA Image Rejection Verification Test Frequencies

Start Frequency	Stop Frequency (GHz)	Step Size (MHz)
100.033325 MHz	2.000033325	400
2.399966675 GHz	13.999966675	400

- Commit the PXIe-5665 settings to hardware.
- For each test frequency from Table 26 or Table 27, calculate PXIe-5665 image frequencies using the following formulas:

For test frequencies <3.6 GHz,

- $IF1 \text{ Image} = \text{Test Frequency} + 9.225 \text{ GHz}$
- $IF2 \text{ Image} = 3.3875 \text{ GHz}$
- $IF3 \text{ Image} = 987.5 \text{ MHz}$
- $IF2 \text{ Image at RF} = \text{Test Frequency} + 1.225 \text{ GHz}$
- $IF3 \text{ Image at RF} = | \text{Test Frequency} - 375 \text{ MHz} |$ (Evaluated only for images greater than 10 MHz)

For test frequencies > 3.6 GHz,

- $IF1 \text{ Image} = \text{Test Frequency} + 1.225 \text{ GHz}$
- $IF2 \text{ Image} = 987.5 \text{ MHz}$
- $IF2 \text{ Image at RF} = \text{Test Frequency} - 375 \text{ MHz}$

where *Test Frequency* is the PXIe-5665 center frequency.

- For each image and test frequency in the list from step 7 and the PXIe-5665 center frequency from step 5, set the RF source 2 to the frequency with a *Power Setting* of 0 dB. The *RF Source Power Direct* for this frequency is used in step 11.



Note *RF Source Power Direct* value was measured in the [Characterizing RF Source Power \(Direct\)](#) equipment characterization procedure.

9. Wait for 200 ms to allow the PXIe-5665 and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the [Test Equipment](#) section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

10. Acquire the spectrum and determine the peak power for each frequency. The peak power value is the *Measured Level*.
11. For each *Measured Level*, calculate the *Response Correction* using the following equation:

$$\text{Response Correction} = \text{Measured Level} + \text{RF Source Power Direct}$$

12. Calculate the *Image Rejection* at each of the image frequencies using the following equation:

$$\text{Image Rejection} = \text{Response Correction (at test frequency)} - \text{Response Correction (at each image frequency)}$$

13. Repeat steps 5 to 12 for all center frequencies in Table 26 or Table 27.
14. Compare the *Image Rejection* results to the verification test limits in Table 28.

Table 28. Image Rejection Verification Test Limits

Center Frequency	As-Found Limit	As-Left Limit*
100 MHz to 2.2 GHz	-80 dBc	-83 dBc
>2.2 GHz to 3.6 GHz	-77 dBc	-80 dBc
>3.6 GHz to 14 GHz†	-80 dBc	-82 dBc

* Refer to the [As-Found and As-Left Limits](#) section of this document for more information about as-left limits.

† Center frequencies >3.6 GHz apply only to the PXIe-5665 14 GHz VSA.

15. Close the PXIe-5665 session.


If the image rejection verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

Verifying Third-Order Intermodulation Distortion

Frequencies ≤ 700 MHz

1. Connect RF source 1 and RF source 2 to the PXIe-5665 RF IN connector through the anti-distortion test fixture as shown in Figure 19 and Figure 20.


Figure 19. PXIe-5665 3.6 GHz VSA Third-Order Intermodulation Verification (Frequencies ≤ 700 MHz) Equipment Setup

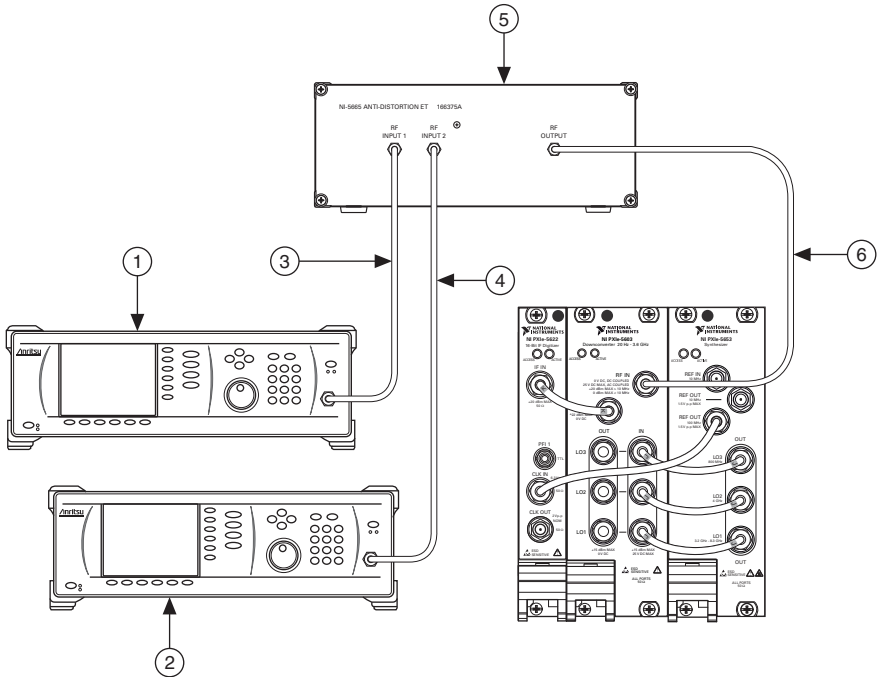

- 1 RF Source 1
- 2 RF Source 2
- 3 SMA (m)-to-SMA (m) cable

- 4 SMA (m)-to-SMA (m) cable
- 5 Anti-Distortion Test Fixture
- 6 SMA (m)-to-SMA (m) cable

**Figure 20. PXIe-5665 14 GHz VSA Third-Order Intermodulation Verification
(Frequencies ≤ 700 MHz) Equipment Setup**

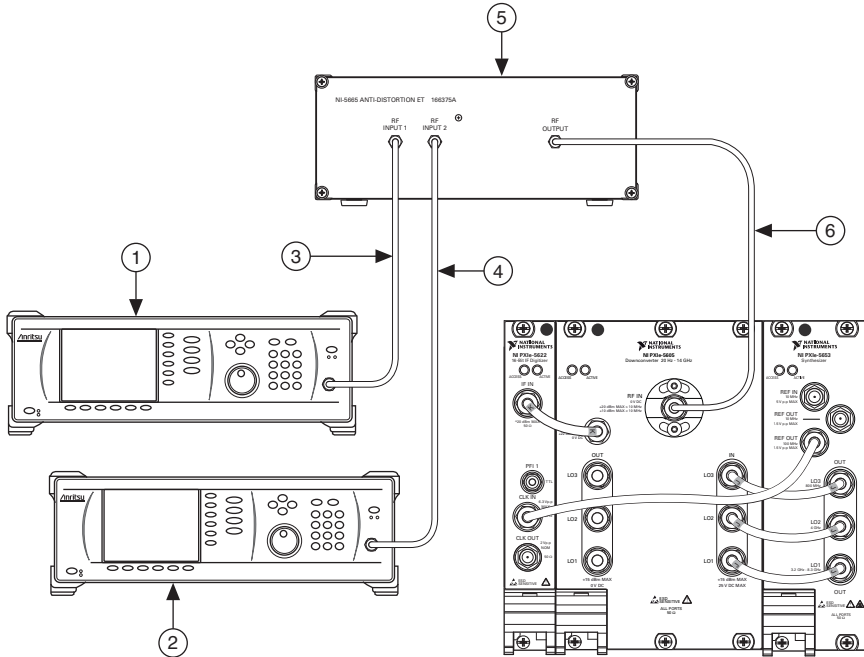

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) cable | 6 SMA (m)-to-SMA (m) cable |

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 10
 - Digital IF Equalization Enabled: TRUE
 - Digitizer Dither Enabled: Enabled
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - RF Attenuation: 0 dB
 - Device Instantaneous Bandwidth: 300 kHz
 - IF Output Power Level: 0 dB
 - Resolution Bandwidth: 750 Hz
 - Span: 150 kHz
4. Configure the anti-distortion test fixture to use the ≤ 700 MHz combiner path.

5. Disable the RF source 1 and RF source 2 outputs.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

6. Set the RF source 1 power to the *RF Source 1 Programmed Power*¹ corresponding to one of the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
7. Set the RF source 2 power to the *RF Source 2 Programmed Power*² corresponding to one of the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
8. Configure the PXIe-5665 reference level to one of the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
9. For each test frequency from Table 29, calculate the following four frequencies:
 - *IMD Low Frequency* = *Test Frequency* - 1.05 MHz
 - *P1 Frequency* = *Test Frequency* + 350 kHz
 - *P2 Frequency* = *Test Frequency* - 350 kHz
 - *IMD High Frequency* = *Test Frequency* + 1.05 MHz
 where *IMD* is the intermodulation distortion.

Table 29. TOI (Frequencies ≤700 MHz) Verification Test Frequencies

Start Frequency	Stop Frequency (MHz)	Step Size (MHz)
12.05 MHz	92.05	40
100 MHz	700	300

10. Set the RF source 1 frequency to *P1 Frequency*.
11. Set the RF source 2 frequency to *P2 Frequency*.
12. Set the PXIe-5665 center frequency to *IMD Low Frequency*.
13. Commit the PXIe-5665 settings to hardware.
14. Enable the RF source 1 and the RF source 2 outputs.

¹ The *RF Source 1 Programmed Power* value was measured in the *RF Source Power (Combined) for Frequencies ≤ 700 MHz* equipment characterization procedure.

² The *RF Source 2 Programmed Power* value was measured in the *RF Source Power (Combined) for Frequencies ≤ 700 MHz* equipment characterization procedure.

15. Wait 2.5 s before making the first measurement and wait 100 ms before making subsequent measurements to allow the PXIe-5665, RF source 1, and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the [Test Equipment](#) section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

16. Measure the power spectrum with the PXIe-5665.
17. Find the highest peak within the measurement bandwidth. This value is the *IMD Low Power*.
18. Repeat steps 11 to 16 for the PXIe-5665 center frequencies of *P1 Frequency*, *P2 Frequency*, and *IMD High Frequency*. The values from step 16 are *IMD Low Power*, *P1 Power*, *P2 Power*, and *IMD High Power*, respectively.
19. Calculate the upper and lower third-order intercept (TOI) points using the following equations:

$$TOI\ Upper = P1\ Power + (P2\ Power - IMD\ High\ Power)/2$$

$$TOI\ Lower = P2\ Power + (P1\ Power - IMD\ Low\ Power)/2$$

20. The smaller of the *TOI Lower* and *TOI Upper* values is the *TOI Minimum*.
21. Repeat steps 8 to 19 for all test frequencies in Table 29.
22. Repeat steps 5 to 20 with the PXIe-5665 preamplifier enabled.
23. Compare the *TOI Minimum* to the verification test limits in Table 30 or Table 31 as appropriate.

Table 30. TOI (Frequencies ≤700 MHz) Verification Test Limits (Preamplifier Disabled)

Center Frequency	As-Found Limit (dBm)	As-Left Limit (dBm)*
10 MHz to <100 MHz	+16	+17
100 MHz to 700 MHz	+19	+20

* Refer to the [As-Found and As-Left Limits](#) section of this document for more information about as-left limits.

Table 31. TOI (Frequencies ≤700 MHz) Verification Test Limits (Preamplifier Enabled)

Center Frequency	As-Found Limit (dBm)	As-Left Limit (dBm)*
10 MHz to <100 MHz	-3	-2
100 MHz to 700 MHz	+2	+3

* Refer to the [As-Found and As-Left Limits](#) section of this document for more information about as-left limits.

24. Disable the output of the RF source 1 and RF source 2.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.


25. Close the PXIe-5665 session.

If the third-order intermodulation distortion for frequencies ≤ 700 MHz verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

Frequencies >700 MHz


1. Connect RF source 1 and RF source 2 to the PXIe-5665 RF IN connector through the anti-distortion test fixture as shown in Figure 21 and Figure 22.

Figure 21. PXIe-5665 3.6 GHz VSA Third-Order Intermodulation (Frequencies >700 MHz) Verification Equipment Setup

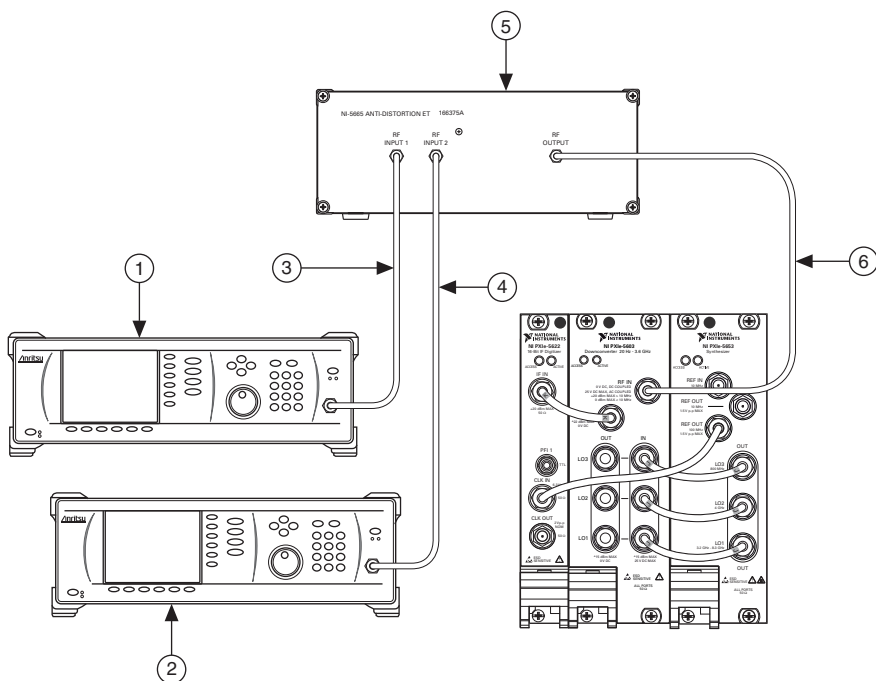

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) cable | 6 SMA (m)-to-SMA (m) cable |

Figure 22. PXIe-5665 14 GHz VSA Third-Order Intermodulation (Frequencies >700 MHz) Verification Equipment Setup

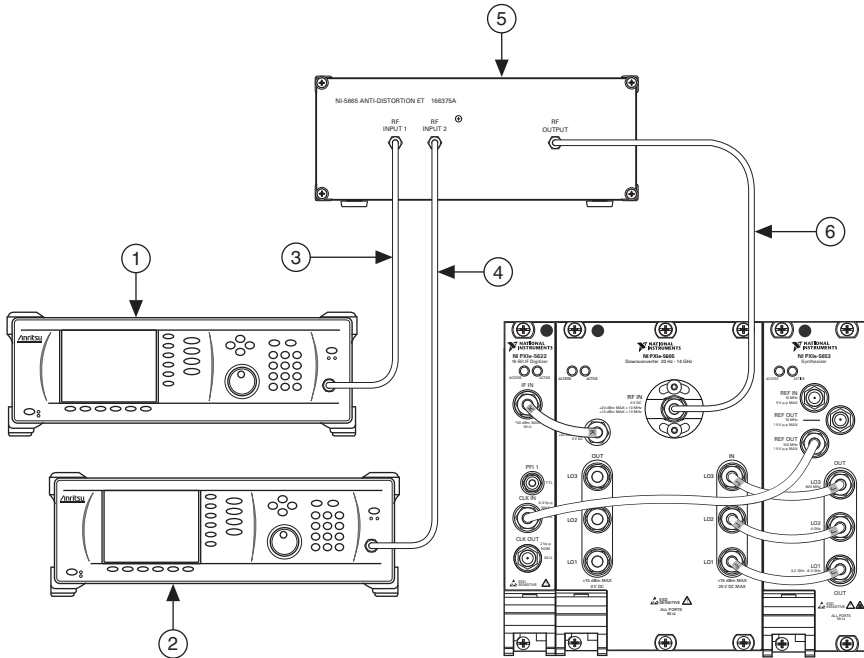

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) cable | 6 SMA (m)-to-SMA (m) cable |

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: RMS Averaging
 - Number of Averages: 10
 - Digital IF Equalization Enabled: TRUE
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - RF Attenuation: 0 dB
 - Device Instantaneous Bandwidth: 300 kHz
 - IF Output Power Level: 0 dB
 - Resolution Bandwidth: 750 Hz
 - Span: 150 kHz
 - **(PXIe-5665 14 GHz VSA) Preselector Enabled: Disabled**
4. Configure the anti-distortion test fixture to use the >700 MHz combiner path.

- Disable the RF source 1 and RF source 2 outputs.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

- Set the RF source 1 power to the *RF Source 1 Programmed Power*¹ corresponding to one of the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
- Set the RF source 2 power to the *RF Source 2 Programmed Power*² corresponding to one of the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
- Configure the PXIe-5665 Reference Level to one the following values:
 - Preamplifier disabled: -10 dBm
 - Preamplifier enabled: -30 dBm
- For each test frequency from Table 32 or Table 33, calculate the following four frequencies:
 - IMD Low Frequency* = Test Frequency - 1.05 MHz
 - P1 Frequency* = Test Frequency + 350 kHz
 - P2 Frequency* = Test Frequency - 350 kHz
 - IMD High Frequency* = Test Frequency + 1.05 MHz

Table 32. PXIe-5665 3.6 GHz VSA TOI (Frequencies >700 MHz)
Verification Test Frequencies

Start Frequency	Stop Frequency	Step Size
800 MHz	3.3 GHz	500 MHz
3.59895 GHz	—	—

¹ The *RF Source 1 Programmed Power* value was measured in the *Characterizing RF Source Power (Combined) for Frequencies >700 MHz* equipment characterization procedure.

² The *RF Source 2 Programmed Power* value was measured in the *Characterizing RF Source Power (Combined) for Frequencies >700 MHz* equipment characterization procedure.

Table 33. PXIe-5665 14 GHz VSA TOI (Frequencies >700 MHz)
Verification Test Frequencies

Preamp Enabled	Start Frequency	Stop Frequency (GHz)	Step Size (MHz)
Enabled	800 MHz	3.3	500
Disabled	800 MHz	3.3	500
	3.6 GHz	13.6	500
	13.99895 GHz	—	—

10. Set the RF source 1 frequency to *P1 Frequency*.
11. Set the RF source 2 frequency to *P2 Frequency*.
12. Set the PXIe-5665 center frequency to *IMD Low Frequency*.
13. Commit the PXIe-5665 settings to hardware.
14. Enable the RF source 1 and RF source 2 outputs.
15. Wait 2.5 s before making the first measurement and wait 100 ms before making subsequent measurements to allow the PXIe-5665, RF source 1, and RF source 1 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the [Test Equipment](#) section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

16. Measure the power spectrum with the PXIe-5665.
17. Find the highest peak within the measurement bandwidth. This value is the *IMD Low Power*.
18. Repeat steps 11 to step 16 for the PXIe-5665 center frequencies of *P1 Frequency*, *P2 Frequency*, and *IMD High Frequency*. The values from step 16 are *IMD Low Power*, *P1 Power*, *P2 Power*, and *IMD High Power*, respectively.
19. Calculate the upper and lower TOI points using the following equations:

$$TOI\ Upper = P1\ Power + (P2\ Power - IMD\ High\ Power)/2$$

$$TOI\ Lower = P2\ Power + (P1\ Power - IMD\ Low\ Power)/2$$

The smaller value of the *TOI Lower* and *TOI Upper* is the *TOI Minimum*.

20. Repeat steps 8 to 18 for all test frequencies in Table 32.
21. Repeat steps 5 to 19 with the PXIe-5665 preamplifier enabled for frequencies greater than or equal to 3.6 GHz.

22. Compare the *TOI Minimum* to the verification test limits in Table 34 or Table 35 as appropriate.

Table 34. TOI (Frequencies >700 MHz) Verification Test Limits (Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Disabled)

Center Frequency	As-Found Limit (dBm)	As-Left Limit (dBm)*
>700 MHz to 3.6 GHz	+20	+21
>3.6 GHz to 14 GHz†	+20	+21
<p>* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.</p> <p>† Center frequencies >3.6 GHz apply only to the PXIe-5665 14 GHz VSA.</p>		

Table 35. TOI (Frequencies >700 MHz) Verification Test Limits (Preamplifier Enabled)

Center Frequency	As-Found Limit	As-Left Limit*
>700 MHz to 3.6 GHz	+2.5 dBm	+3.5 dBm
<p>* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.</p>		

23. Disable the output of the RF source 1 and RF source 2.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.


24. Close the PXIe-5665 session.

If the third-order intermodulation distortion for frequencies >700 MHz verification procedure determines that the PXIe-5665 is outside its limits, refer to *Worldwide Support and Services* for information about support resources or service requests.

Verifying Second Harmonic Intercept (SHI)


1. Connect RF source 1 and RF source 2 to the PXIe-5665 RF IN connector through the anti-distortion test fixture as shown in Figure 23 and Figure 24.

Figure 23. PXIe-5665 3.6 GHz VSA SHI Verification Equipment Setup

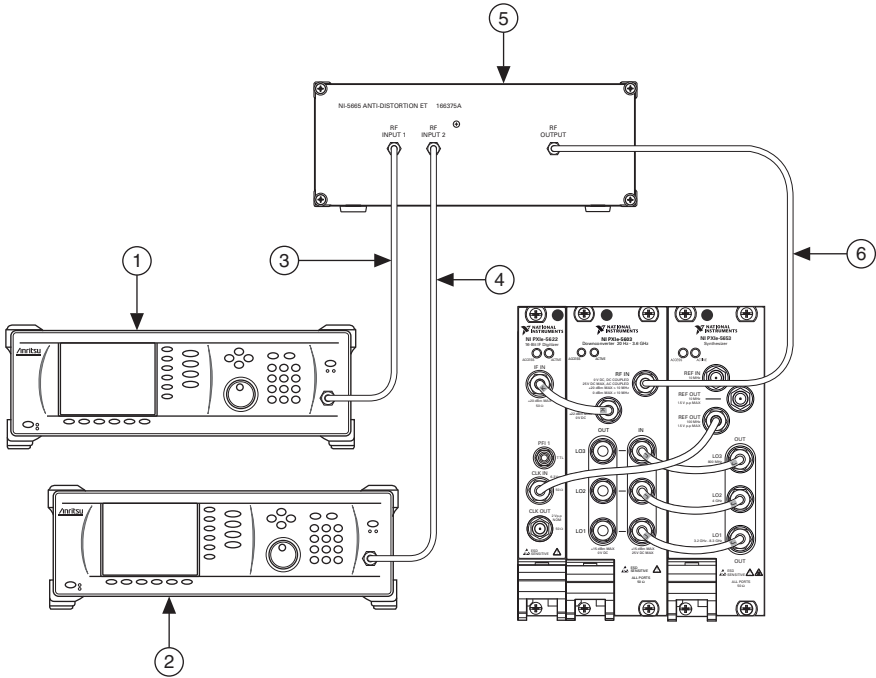

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) Cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) Cable | 6 SMA (m)-to-SMA (m) Cable |

Figure 24. PXIe-5665 14 GHz VSA SHI Verification Equipment Setup

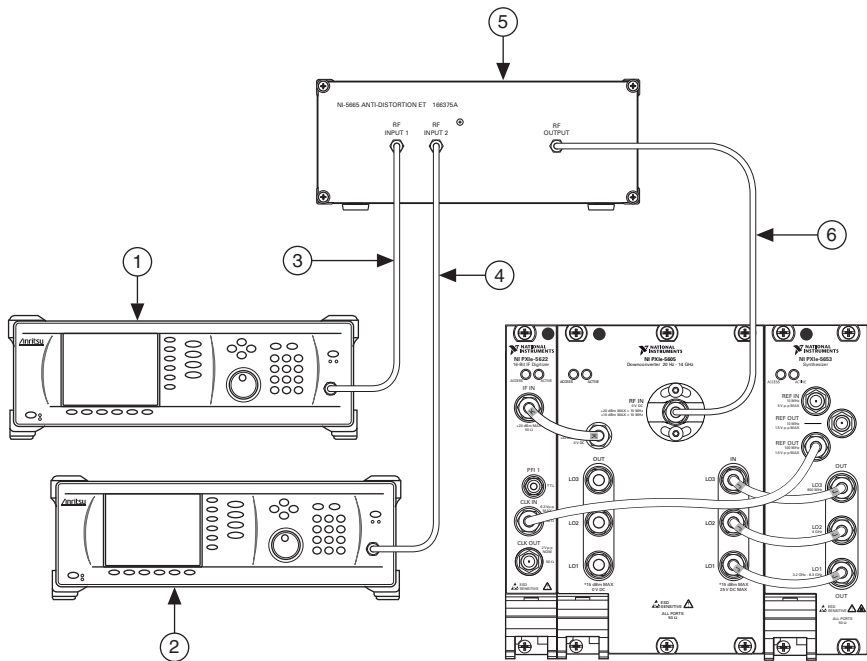

- | | |
|---|---|
| <p>1 RF Source 1</p> <p>2 RF Source 2</p> <p>3 SMA (m)-to-SMA (m) Cable</p> | <p>4 SMA (m)-to-SMA (m) Cable</p> <p>5 Anti-Distortion Test Fixture</p> <p>6 SMA (m)-to-SMA (m) Cable</p> |
|---|---|

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Digital IF Equalization Enabled: TRUE
 - Digitizer Dither Enabled: Enabled
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - Span: 150 kHz
 - Device Instantaneous Bandwidth: 300 kHz
 - Resolution Bandwidth: 750 Hz
 - RF Attenuation: 10 dB
 - Power Spectrum Units: Volts Squared
 - **(PXIe-5665 14 GHz VSA) Preselector Enabled: Disabled**
4. Configure the anti-distortion test fixture to use the 470 MHz Lowpass Filter path.

5. Disable the RF source 1 and RF source 2 outputs.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

6. Disable the PXIe-5665 preamplifier.
7. Set the PXIe-5665 reference level to one of the following values:
 - Preamplifier disabled: 0 dBm
 - Preamplifier enabled: -30 dBm
8. Set the RF source 2 frequency and the PXIe-5665 center frequency to the values shown in the first row of Table 36.

Table 36. SHI Verification Test Frequencies

Start Frequency	Stop Frequency	Step Size (MHz)
300 MHz	700 MHz	200
800 MHz	1.8 GHz	500
2 GHz	3.5 GHz	500
3.8 GHz	6.8 GHz	500
7 GHz	—	—

9. Configure the anti-distortion test fixture to use the appropriate Lowpass Filter Path as shown in Table 37.

Table 37. Lowpass Filter Specifications

Lowpass Filter Path (MHz)	Frequency Range
470	1 MHz to 470 MHz
735	>470 MHz to 735 MHz
1,150	>735 MHz to 1.150 GHz
1,800	>1.150 GHz to 1.800 GHz
2,530	>1.800 GHz to 2.530 GHz
3,550	>2.530 GHz to 3.550 GHz
4,985	>3.550 GHz to 4.985 GHz
7,000	>4.985 GHz to 7.000 GHz

10. Commit the PXIe-5665 settings to hardware.

11. Set the RF source 2 power to the *RF Source Power LPF* to one of the following values for the RF source 2 frequency:
 - Preamplifier disabled: 0 dBm
 - Preamplifier enabled: -30 dBm
12. Enable the RF source 2 output.
13. Wait 500 ms before making the first measurement and wait 100 ms before making subsequent measurements to allow the PXIe-5665 and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the *Test Equipment* section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

14. Measure the power spectrum with the PXIe-5665.
15. Find the highest peak within the measurement bandwidth (BW). This value is the *Peak Power*.
16. Calculate the *Noise Measurement BW* and the *Noise Center Frequency (CF)* using the following equations:

$$\text{Noise Measurement BW} = \frac{\text{Span}}{2} - \frac{10 \text{ kHz}}{2}$$

$$\text{Noise CF} = \text{Center Frequency} + \frac{\text{Span}}{4} + \frac{10 \text{ kHz}}{4}$$

17. Calculate the *Power in Band* for the spectrum from step 13 using the *Noise Measurement BW* and *Noise CF* values from step 16.



Note *Power in Band* is a built-in function in the NI Spectral Measurements Toolkit.

18. Calculate the *Average Noise Power* using the following equation:

$$\text{Average Noise Power} = \text{Power in Band} - 10 \log_{10} \left(\frac{\text{Noise Measurement BW}}{\text{Resolution Bandwidth}} \right)$$

19. Record either *Peak Power* (from step 14) or *Average Noise Power* (from step 17). According to the frequency tuned to with the PXIe-5665, record whichever value is greater as the *Fundamental Power* or the *Harmonic Power*.
20. Repeat steps 7 to 19 for the second harmonic, which is twice the test frequency.
21. Calculate the SHI using the following equation:

$$\text{SHI} = 2(\text{Fundamental Power}) - \text{Harmonic Power} - \text{RF Attenuation}$$

22. Repeat steps 7 to 20 for all test frequencies listed in Table 36.

23. **(PXIe-5665 14 GHz VSA)** Repeat steps 6 to 21 for test frequencies between 3.8 GHz and 7 GHz with the PXIe-5665 preselector enabled.
24. Repeat steps 6 to 22 for the frequencies in Table 38 with the PXIe-5665 preamplifier enabled.

Table 38. SHI Verification Test Frequencies

Start Frequency (MHz)	Stop Frequency	Step Size
300.0333125	1.3000333125 GHz	200 MHz
1,800	—	—

25. Compare the *SHI* to the verification test limits in Table 39, Table 40, or Table 41 as appropriate.

Table 39. SHI Verification Test Limits (Preamplifier Disabled, PXIe-5665 14 GHz VSA Preselector Enabled)

Source Frequency	Device	As-Found Limit (dBm)	As-Left Limit (dBm)*
300 MHz to <700 MHz	PXIe-5665	+42	+43
700 MHz to 1.8 GHz	PXIe-5665 3.6 GHz VSA	+50	+51
	PXIe-5665 14 GHz VSA	+44	+45
>1.8 GHz to 3.75 GHz†	PXIe-5665 14 GHz VSA	+54	+56
>3.75 GHz to 4.25 GHz†		+54	+56
>4.25 GHz to 7 GHz†		+54	+56
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.			
† Source frequencies >1.8 GHz apply only to the PXIe-5665 14 GHz VSA.			

Table 40. SHI Verification Test Limits (Preamplifier Enabled)

Source Frequency	Device	As-Found Limit (dBm)	As-Left Limit (dBm)*
300 MHz to 1.8 GHz	PXIe-5665 3.6 GHz VSA	+15	+18
	PXIe-5665 14 GHz VSA	+20	+25
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.			

Table 41. SHI Verification Test Limits (PXIe-5665 14 GHz VSA Preselector Disabled)

Frequency (GHz)	As-Found Limit (dBm)	As-Left Limit (dBm)*
>1.80 to 4.25	+28	+30
>4.25 to 7.00	+18	+20
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.		

26. Disable the output of RF source 2.



Note When disabled, the RF source 2 output signal should be less than -60 dBm.

27. Close the PXIe-5665 session.

If the second harmonic intercept verification procedure determines that the PXIe-5665 is outside its limits, refer to *Worldwide Support and Services* for information about support resources or service requests.

Verifying Gain Compression

This procedure verifies that <1 dB of gain compression occurs when the specified power level is applied at the RF IN connector of the PXIe-5665.




Note The power level you apply differs whether you are verifying the as-found or as-left limit.

Frequencies ≤ 700 MHz

1. Connect RF source 1 and RF source 2 to the PXIe-5665 RF IN connector through the anti-distortion test fixture, as shown in Figure 25 and Figure 26.


Figure 25. PXIe-5665 3.6 GHz VSA Gain Compression Verification (Frequencies ≤ 700 MHz) Equipment Setup

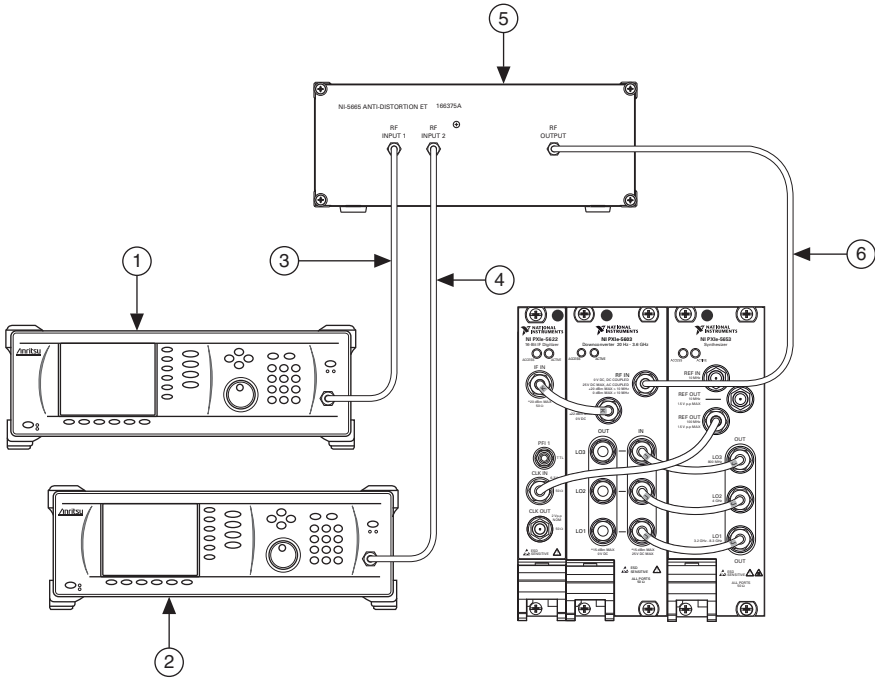

- 1 RF Source 1
- 2 RF Source 2
- 3 SMA (m)-to-SMA (m) Cable

- 4 SMA (m)-to-SMA (m) Cable
- 5 Anti-Distortion Test Fixture
- 6 SMA (m)-to-SMA (m) Cable

**Figure 26. PXIe-5665 14 GHz VSA Gain Compression Verification
(Frequencies ≤ 700 MHz) Equipment Setup**

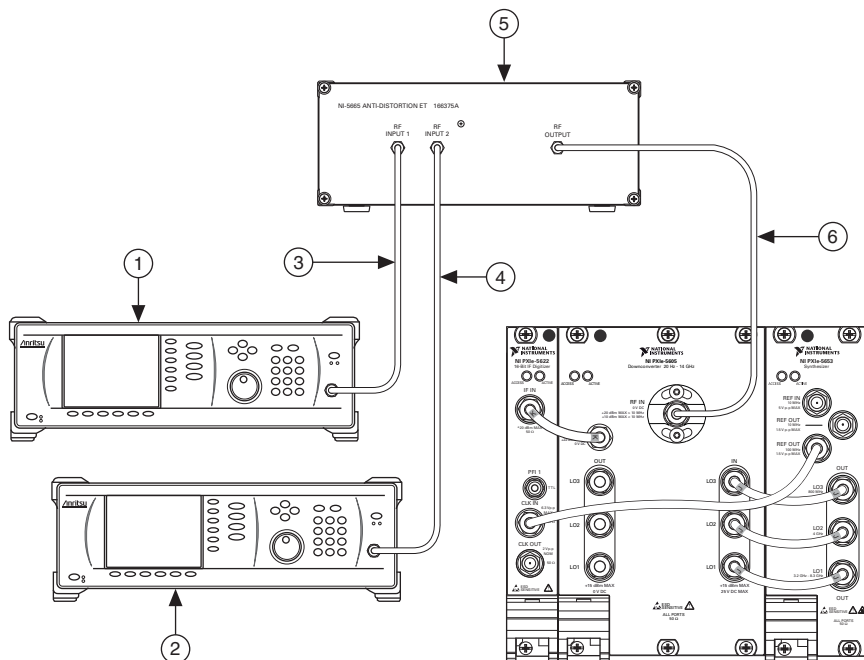

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) Cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) Cable | 6 SMA (m)-to-SMA (m) Cable |

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: No Averaging
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - Span: 100 kHz
 - Device Instantaneous Bandwidth: 300 kHz
 - Resolution Bandwidth: 500 Hz
 - RF Attenuation: 0 dB
 - FFT Window Type: Flat Top
4. Configure the anti-distortion test fixture to use the ≤ 700 MHz combiner path.

5. Disable the RF source 1 and RF source 2 outputs.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

6. Disable the PXIe-5665 preamplifier.
7. Set the RF source 2 frequency according to Table 42.
8. Set the RF source 1 frequency 1 MHz above the RF source 2 frequency.
9. Set the PXIe-5665 center frequency according to the first row in Table 42.

Table 42. Gain Compression Verification Test Frequencies (Frequencies ≤ 700 MHz)

Start Frequency (MHz)	Stop Frequency (MHz)	Step Size (MHz)
10	90	40
100	700	200

10. Set the RF source 2 power to the *RF Source 2 Programmed Power* in Table 43 or Table 44 as appropriate.
11. Set the RF source 1 power to the *RF Source 1 Programmed Power* in Table 43 or Table 44 as appropriate.
12. Set the PXIe-5665 reference level according to Table 43 or Table 44 as appropriate.

Table 43. Gain Compression Verification Test Settings (Preamplifier Disabled)

Setting	Frequency Range (MHz)	Limit	Value (dBm)
RF Source 1 Programmed Power	11 to 701	As-Found	+8.0
		As-Left*	+9.1
RF Source 2 Programmed Power	10 to 700	Both	-24
PXIe-5665 Reference Level	10 to 700	Both	0

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

Table 44. Gain Compression Test Settings (Preamplicifier Enabled)

Setting	Frequency Range (MHz)	Limit	Value (dBm)
RF Source 1 Programmed Power	11 to 101	As-Found	-18
		As-Left*	-16
	>101 to 701	As-Found	-15
		As-Left*	-13
RF Source 2 Programmed Power	10 to 700	Both	-54
PXIe-5665 Reference Level	10 to 700	Both	-30
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.			

13. Commit the PXIe-5665 settings to hardware.
14. Enable the RF source 2 output and wait 250 ms, or wait 100 ms if the output is already enabled. This wait time allows the PXIe-5665 and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the *Test Equipment* section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

15. Read the power spectrum from the PXIe-5665.
16. Depending on your equipment configuration, using the spectrum returned from the PXIe-5665, measure the power at the center frequency and record this value as the *Small Tone First Measurement* (RF source 1 output disabled) or as the *Small Tone Second Measurement* (RF source 1 output enabled).
17. Repeat steps 7 to 16 for all test frequencies in Table 42.
18. Repeat steps 7 to 17 with the PXIe-5665 preamplifier enabled.
19. Enable the RF source 1 output.
20. Repeat steps 6 to 18 with the RF source 1 output enabled.
21. Calculate the PXIe-5665 *Gain Compression* using the following equation:

$$\text{Gain Compression} = \text{Small Tone First Measurement} - \text{Small Tone Second Measurement}$$

22. Compare the *Gain Compression* to the verification test limits in Table 45 or Table 46 as appropriate.

Table 45. Gain Compression Verification Test Limits
(Frequencies ≤ 700 MHz, Preamplifier Disabled)

Frequency	Limit	Compression (dB)	Applied Power (dBm)
10 MHz to 700 MHz	As-Found	1	+8
	As-Left*	1	+9.1

* Refer to the [As-Found and As-Left Limits](#) section of this document for more information about as-left limits.

The device specification calls for less than or equal to 1 dB gain compression for a minimum applied power. The applied power includes the measurement uncertainty to guarantee the required minimum applied power.

Table 46. Gain Compression Verification Test Limits
(Frequencies ≤ 700 MHz, Preamplifier Enabled)

Frequency	Limit	Compression (dB)	Applied Power (dBm)
10 MHz to 100 MHz	As-Found	1	-18
	As-Left*	1	-16
>100 MHz to 700 MHz	As-Found	1	-15
	As-Left*	1	-13

* Refer to the [As-Found and As-Left Limits](#) section of this document for more information about as-left limits.

The device specification calls for less than or equal to 1 dB gain compression for a minimum applied power. The applied power includes the measurement uncertainty to guarantee the required minimum applied power.

23. Disable the output of RF source 1 and RF source 2.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.


24. Close the PXIe-5665 session.

If the gain compression for frequencies ≤ 700 MHz verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

Frequencies >700 MHz


1. Connect RF source 1 and RF source 2 to the PXIe-5665 RF IN connector through the anti-distortion test fixture, as shown in Figure 27 and Figure 28.

Figure 27. PXIe-5665 3.6 GHz VSA Gain Compression Verification (Frequencies >700 MHz) Equipment Setup

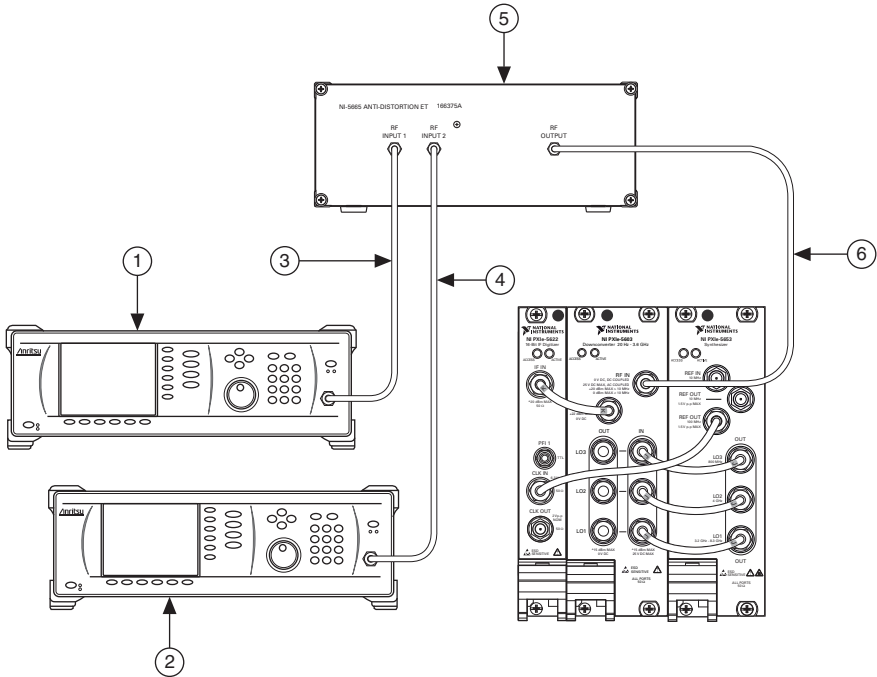

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) Cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) Cable | 6 SMA (m)-to-SMA (m) Cable |

Figure 28. PXIe-5665 14 GHz VSA Gain Compression Verification
(Frequencies >700 MHz) Equipment Setup

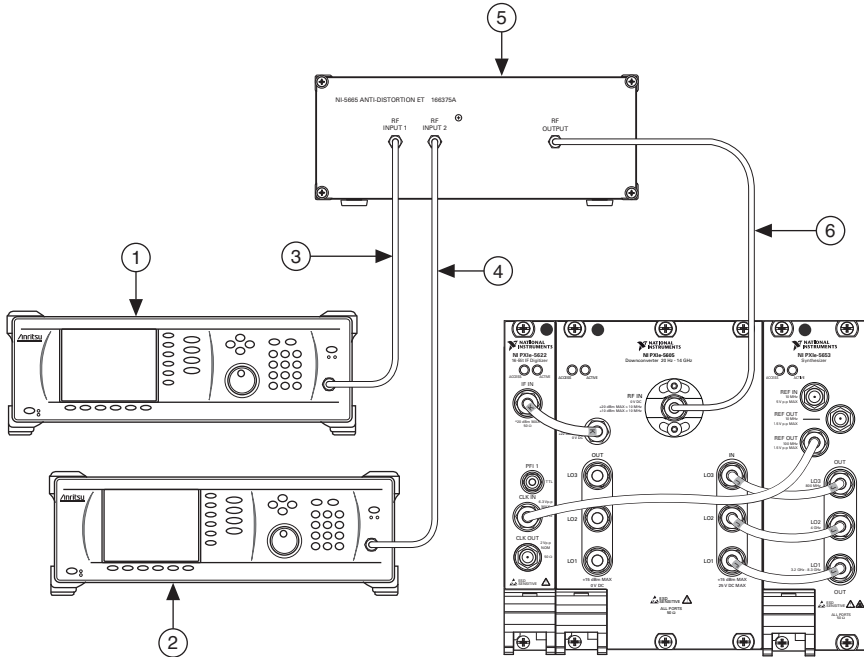

- | | |
|----------------------------|--------------------------------|
| 1 RF Source 1 | 4 SMA (m)-to-SMA (m) Cable |
| 2 RF Source 2 | 5 Anti-Distortion Test Fixture |
| 3 SMA (m)-to-SMA (m) Cable | 6 SMA (m)-to-SMA (m) Cable |

2. Create a new session for the PXIe-5665.
3. Configure the PXIe-5665 according to the following property settings:
 - Acquisition Type: Spectrum
 - Averaging Mode: No Averaging
 - Ref Clock Source: PXI_Clk
 - Channel Coupling: AC Coupled
 - Span: 100 kHz
 - Device Instantaneous Bandwidth: 300 kHz
 - Resolution Bandwidth: 500 Hz
 - RF Attenuation: 0 dB
 - FFT Window Type: Flat Top
4. Configure the anti-distortion test fixture to use the >700 MHz combiner path.

5. Disable the RF source 1 and RF source 2 outputs.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

6. Disable the PXIe-5665 preamplifier.
7. **(PXIe-5665 14 GHz VSA)** Disable the PXIe-5665 preselector.
8. Set the RF source 2 frequency according to the first row in Table 47 or Table 48 as appropriate.

Table 47. PXIe-5665 3.6 GHz Gain Compression Test Frequencies
(Frequencies >700 MHz)

Start Frequency	Stop Frequency	Step Size
800 MHz	3.3 GHz	500 MHz
3.6 GHz	—	—

Table 48. PXIe-5665 14 GHz Gain Compression Test Frequencies
(Frequencies >700 MHz)

Start Frequency	Stop Frequency	Step Size
800 MHz	3.3 GHz	500 MHz
3.6 GHz	—	—
3.8 GHz	13.8 GHz	500 MHz
14 GHz	—	—

9. Set the RF source 1 frequency 1 MHz above the RF source 2 frequency.
10. Set the PXIe-5665 center frequency according to the values listed in Table 47 or Table 48.
11. Set the RF source 2 power to the *RF Source 2 Programmed Power* from Table 49 or Table 50 as appropriate.
12. Set the RF source 1 power to the *RF Source 1 Programmed Power* from Table 49 or Table 50 as appropriate.

13. Set the PXIe-5665 reference level according to Table 49 or Table 50 as appropriate.

**Table 49. Gain Compression Verification Test Settings
(Preamplifier Disabled)**

Device	Setting	Frequency Range	Limit	Value (dBm)
PXIe-5665 3.6 GHz VSA	RF Source 1 Programmed Power	801 MHz to 1.701 GHz	As-Found	+8.0
			As-Left*	+9.1
		>1.701 GHz to 3.601 GHz	As-Found	+6.0
			As-Left*	+7.1
	RF Source 2 Programmed Power	800 MHz to 3.600 GHz	Both	-24
PXIe-5665 Reference Level	800 MHz to 3.600 GHz	Both	0	
PXIe-5665 14 GHz VSA	RF Source 1 Programmed Power	801 MHz to 1.701 GHz	As-Found	+8.0
			As-Left*	+9.1
		>1.701 GHz to 14.001 GHz	As-Found	+6.0
			As-Left*	+7.1
	RF Source 2 Programmed Power	800 MHz to 14.00 GHz	Both	-24
PXIe-5665 Reference Level	800 MHz to 14.00 GHz	Both	0	
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.				

Table 50. Gain Compression Verification Test Settings
(Preamplifier Enabled)

Device	Setting	Frequency Range	Limit	Value (dBm)
PXIe-5665 3.6 GHz VSA	RF Source 1 Programmed Power	801 MHz to 1.701 GHz	As-Found	-15
			As-Left*	-13
		>1.701 GHz to 3.601 GHz	As-Found	-18
			As-Left*	-16
	RF Source 2 Programmed Power	800 MHz to 3.600 GHz	Both	-54
PXIe-5665 Reference Level	800 MHz to 3.600 GHz	Both	-30	
PXIe-5665 14 GHz VSA	RF Source 1 Programmed Power	801 MHz to 1.701 GHz	As-Found	-15
			As-Left*	-13
		>1.701 GHz to 14.001 GHz	As-Found	-18
			As-Left*	-16
	RF Source 2 Programmed Power	800 MHz to 14.00 GHz	Both	-54
PXIe-5665 Reference Level	80 MHz to 14.00 GHz	Both	-30	
* Refer to the <i>As-Found and As-Left Limits</i> section of this document for more information about as-left limits.				

14. Commit the PXIe-5665 settings to hardware.
15. Enable the RF source 2 output and wait 250 ms, or wait 100 ms if the output is already enabled. This wait time allows the PXIe-5665 and RF source 2 amplitudes to settle.



Note Settling times are a characteristic of the RF source device. Refer to the *Test Equipment* section of this document for a list of NI-recommended source devices and device specifications. If you use an RF source device with different device specifications, your settling times may differ from those listed in this procedure.

16. Read the power spectrum from the PXIe-5665.

17. Depending on your equipment configuration, using the spectrum returned from the PXIe-5665, measure the power at the center frequency and record this value as the *Small Tone First Measurement* (RF source 1 output disabled) or as the *Small Tone Second Measurement* (RF source 1 output enabled).
18. Repeat steps 8 to 17 for all test frequencies in step 8.
19. **(PXIe-5665 14 GHz VSA)** Repeat steps 8 to 18 for frequencies greater than 3.6 GHz with the PXIe-5665 preselector enabled.
20. Repeat steps 7 to 18 with the PXIe-5665 preamplifier enabled for frequencies less than 3.6 GHz.
21. Enable the RF source 1 output.
22. Repeat steps 6 to 20 with the RF source 1 output enabled.
23. Calculate the PXIe-5665 *Gain Compression* using the following equation:

$$\text{Gain Compression} = \text{Small Tone First Measurement} - \text{Small Tone Second Measurement}$$

24. Compare the *Gain Compression* to the verification test limits in Table 51 or Table 52.

Table 51. Gain Compression Verification Test Limits (>700 MHz, Preamplifier Disabled)

Frequency	Limit	Compression (dB)	Applied Power (dBm)
>700 MHz to 1.70 GHz	As-Found	1	+8.0
	As-Left*	1	+9.1
>1.70 GHz to 3.6 GHz	As-Found	1	+6.0
	As-Left*	1	+7.1

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

The device specification calls for less than or equal to 1 dB gain compression for a minimum applied power. The applied power includes the measurement uncertainty to guarantee the required minimum applied power.

Table 52. Gain Compression Verification Test Limits (>700 MHz, Preamplifier Enabled)

Frequency	Limit	Compression (dB)	Applied Power (dBm)
>700 MHz to 1.70 GHz	As-Found	1	-15
	As-Left*	1	-13
>1.70 GHz to 3.6 GHz	As-Found	1	-18
	As-Left*	1	-16

* Refer to the *As-Found and As-Left Limits* section of this document for more information about as-left limits.

The device specification calls less than or equal to 1 dB gain compression for a minimum applied power. The applied power includes the measurement uncertainty to guarantee the required minimum applied power.

25. Disable the output of RF source 1 and RF source 2.



Note When disabled, the RF source 1 and RF source 2 output signals should be less than -60 dBm.

26. Close the PXIe-5665 session.

If the gain compression for frequencies >700 MHz verification procedure determines that the PXIe-5665 is outside its limits, refer to *Worldwide Support and Services* for information about support resources or service requests.

Verifying LO Output Power




Note Prior to starting this procedure, zero and calibrate the power sensor according to the *Zeroing and Calibrating the Power Sensor* section of this document.

1. Connect the RF source 2 output to the PXIe-5605 RF IN connector using the SMA (m)-to-SMA (m) cable.
2. Connect power sensor A to the PXIe-5605 LO3 OUT connector using the SMA (m)-to-SMA (m) cable.
3. Connect the spectrum analyzer to the PXIe-5605 LO2 OUT connector.

- Connect power sensor B to the PXIe-5605 LO1 OUT connector. The completed setup is shown in Figure 29 and Figure 30.

Figure 29. PXIe-5665 3.6 GHz VSA LO Output Power Verification Equipment Setup

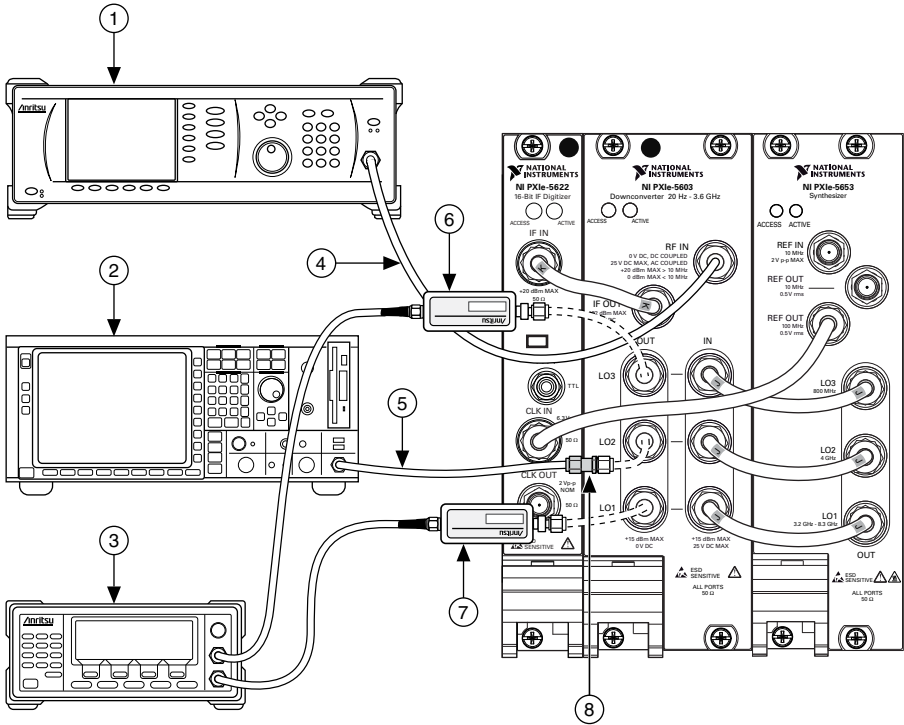


- | | | |
|---------------------|----------------------------|--------------------|
| 1 RF Source 2 | 4 SMA (m)-to-SMA (m) Cable | 7 Power Sensor B |
| 2 Spectrum Analyzer | 5 SMA (m)-to-SMA (m) Cable | 8 10 dB Attenuator |
| 3 Power Meter | 6 Power Sensor A | |



Note Attach the 10 dB attenuator directly to the PXIe-5606 LO2 OUT connector.

Figure 30. PXIe-5665 14 GHz VSA LO Output Power Verification Equipment Setup

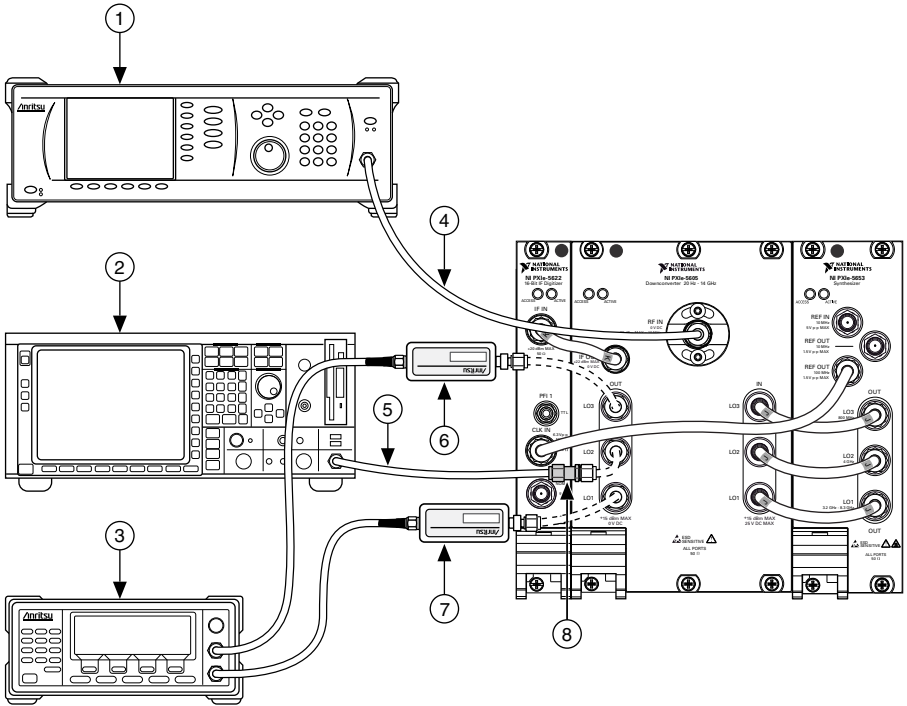

- | | | |
|---------------------|----------------------------|--------------------|
| 1 RF Source 2 | 4 SMA (m)-to-SMA (m) Cable | 7 Power Sensor B |
| 2 Spectrum Analyzer | 5 SMA (m)-to-SMA (m) Cable | 8 10 dB Attenuator |
| 3 Power Meter | 6 Power Sensor A | |



Note Attach the 10 dB attenuator directly to the PXIe-5606 LO2 OUT connector.

5. Configure the spectrum analyzer according to the following settings:
 - Resolution Bandwidth: 1 kHz
 - Span: 0 Hz
 - Reference Level: +20 dBm
 - Center Frequency: 4 GHz
6. Configure the RF source 2 according to the following settings:
 - Power: -20 dBm
 - Frequency: 1 GHz



Note The RF source 2 settings do not affect this test. It is programmed to a known state for convenience only.

7. Create a new session for the PXIe-5665.

8. Configure the PXIe-5665 according to the following property setting:
 - LO Export Enabled: True
9. Initiate the PXIe-5665.
10. Close the PXIe-5665 session.
11. Create a new session for the PXIe-5653.
12. Configure the PXIe-5653 according to the following property settings:
 - Ref Clock Source: PXI -Clk
 - Frequency: 4.05625 GHz
13. Read the power meter channel B power and correct for the PXIe-5653 frequency.
14. Repeat step 13 and record the frequency where the minimum measured power occurs for the following PXIe-5653 frequencies:
 - Minimum frequency: 4.05625 GHz
 - Maximum frequency: 8.2125 GHz
 - Frequency step: 50 MHz
15. Tune the PXIe-5653 to the frequency found in step 14.
16. Measure the LO1 power with power meter channel B. Correct the reading for the LO1 frequency.
17. Measure the LO2 power with the spectrum analyzer. Correct the reading for the 4 GHz LO2 frequency using the following equation:

$$LO2\ Power = Spectrum\ Analyzer\ Reading + Spectrum\ Analyzer\ Correction\ Factor^1$$
18. Measure the LO3 power with power meter channel A. Correct the reading for the LO3 frequency of 800 MHz.
19. Compare the readings from steps 16 to 18 to the following verification test limits in Table 53.

Table 53. LO Output Power Verification Test Limits

LO	As-Found (dBm)	As-Left (dBm)
LO1	>7.0	7.0 to 8.0
LO2	>7.0	9.0 to 10.0
LO3	>7.0	9.0 to 10.0

20. Close the PXIe-5653 session.

If the LO output power verification procedure determines that the PXIe-5665 is outside its limits, refer to [Worldwide Support and Services](#) for information about support resources or service requests.

¹ The *Spectrum Analyzer Correction Factor* value was calculated in the [Characterizing Spectrum Analyzer Response](#) equipment characterization procedure.

Reverification

Repeat the *Verification* section to determine the as-left status of the device.

Appendix A: Anti-Distortion Test Fixture



Note The anti-distortion test fixture specifications are for the entire fixture and include the performance of all components internal to the fixture.

Table 54. Lowpass Filter Passband Paths

Filter Path (MHz)	Start (MHz)	Stop (MHz)	Insertion Loss (dB, max.)	VSWR [*] (max.)
470	10	≤470	2.5	1.75
735	>470	≤735	2.5	1.75
1,150	>735	≤1,150	2.5	1.75
1,800	>1,150	≤1,800	2.5	1.75
2,530	>1,800	≤2,530	2.5	1.75
3,550	>2,530	≤3,550	2.5	1.75
4,985	>3,550	≤4,985	2.5	1.75
7,000	>4,985	≤7,000	2.5	1.75

* Input or output ports.

Table 55. Lowpass Filter Stopband Paths

Filter Path (MHz)	Start (MHz)	Stop (MHz)	Rejection [*]
470	600	≤940	50
735	>940	≤1,470	50
1,150	>1,470	≤2,300	50
1,800	>2,300	≤3,600	50
2,530	>3,600	≤5,060	70
3,550	>5,060	≤7,100	70
4,985	>7,100	≤9,970	70
7,000	>9,970	≤14,000	70

* Rejection equals *Fundamental Power - Second Harmonic Power*

Table 56. Combiner Paths

Combiner	Path	Start	Stop	Total Loss* (dB, max.)	Isolation† (dB, min.)	VSWR‡ (max.)
2	1	>700 MHz	10 GHz	8.0	20	1.75
	2			18.0		
2	1	>10 GHz	14 GHz	8.0	20	2.00
	2			18.0		

* *Total Loss* includes the splitter loss at either input or output ports. The unused input port is terminated in 50 Ω.

† *Isolation* is the loss between input ports. The output port is terminated in 50 Ω.

‡ *VSWR* includes any port. All other ports are terminated in 50 Ω.

Appendix B: Power Sensor Calibration Factor Uncertainty

Table 57. Maximum Power Sensor Calibration Factor Uncertainty

Frequency	Calibration Factor Uncertainty (%)
10 MHz	≤1.15
20 MHz	≤0.80
30 MHz	≤0.65
40 MHz to 200 MHz	≤0.55
300 MHz to 400 MHz	≤0.60
500 MHz to 1 GHz	≤0.50
2 GHz to 4 GHz	≤0.60
5 GHz	≤0.75
6 GHz	≤0.80
7 GHz	≤0.85
8 GHz	≤0.90
9 GHz	≤0.95
10 GHz	≤1.00

Table 57. Maximum Power Sensor Calibration Factor Uncertainty (Continued)

Frequency	Calibration Factor Uncertainty (%)
11 GHz	≤1.05
12 GHz	≤1.10
13 GHz	≤1.15
14 GHz	≤1.20
15 GHz	≤1.25

Worldwide Support and Services

The National Instruments website is your complete resource for technical support. At ni.com/support you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit ni.com/services for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit ni.com/register to register your National Instruments product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

A Declaration of Conformity (DoC) is our claim of compliance with the Council of the European Communities using the manufacturer's declaration of conformity. This system affords the user protection for electromagnetic compatibility (EMC) and product safety. You can obtain the DoC for your product by visiting ni.com/certification. If your product supports calibration, you can obtain the calibration certificate for your product at ni.com/calibration.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world. For telephone support in the United States, create your service request at ni.com/support or dial 512 795 8248. For telephone support outside the United States, visit the Worldwide Offices section of ni.com/niglobal to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.

Refer to the *NI Trademarks and Logo Guidelines* at ni.com/trademarks for more information on National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at ni.com/patents. You can find information about end-user license agreements (EULAs) and third-party legal notices in the readme file for your NI product. Refer to the *Export Compliance Information* at ni.com/legal/export-compliance for the National Instruments global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2011–2017 National Instruments. All rights reserved.