

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.


 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

SC-2040

SC-2040

User Manual

Eight-Channel Simultaneous Sample-and-Hold Accessory

September 1994 Edition

Part Number 371191A-01

**© Copyright 1994 National Instruments Corporation.
All Rights Reserved.**

National Instruments Corporate Headquarters

6504 Bridge Point Parkway

Austin, TX 78730-5039

(512) 794-0100

Technical support fax: (800) 328-2203

(512) 794-5678

Branch Offices:

Australia (03) 879 9422, Austria (0662) 435986, Belgium 02/757.00.20, Canada (Ontario) (519) 622-9310,
Canada (Québec) (514) 694-8521, Denmark 45 76 26 00, Finland (90) 527 2321, France (1) 48 14 24 24,
Germany 089/741 31 30, Italy 02/48301892, Japan (03) 3788-1921, Netherlands 03480-33466, Norway 32-848400,
Spain (91) 640 0085, Sweden 08-730 49 70, Switzerland 056/20 51 51, U.K. 0635 523545

Limited Warranty

The SC-2040 is warranted against defects in materials and workmanship for a period of one year from the date of shipment, as evidenced by receipts or other documentation. National Instruments will, at its option, repair or replace equipment that proves to be defective during the warranty period. This warranty includes parts and labor.

A Return Material Authorization (RMA) number must be obtained from the factory and clearly marked on the outside of the package before any equipment will be accepted for warranty work. National Instruments will pay the shipping costs of returning to the owner parts which are covered by warranty.

National Instruments believes that the information in this manual is accurate. The document has been carefully reviewed for technical accuracy. In the event that technical or typographical errors exist, National Instruments reserves the right to make changes to subsequent editions of this document without prior notice to holders of this edition. The reader should consult National Instruments if errors are suspected. In no event shall National Instruments be liable for any damages arising out of or related to this document or the information contained in it.

EXCEPT AS SPECIFIED HEREIN, NATIONAL INSTRUMENTS MAKES NO WARRANTIES, EXPRESS OR IMPLIED, AND SPECIFICALLY DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. CUSTOMER'S RIGHT TO RECOVER DAMAGES CAUSED BY FAULT OR NEGLIGENCE ON THE PART OF NATIONAL INSTRUMENTS SHALL BE LIMITED TO THE AMOUNT THERETOFORE PAID BY THE CUSTOMER. NATIONAL INSTRUMENTS WILL NOT BE LIABLE FOR DAMAGES RESULTING FROM LOSS OF DATA, PROFITS, USE OF PRODUCTS, OR INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF ADVISED OF THE POSSIBILITY THEREOF. This limitation of the liability of National Instruments will apply regardless of the form of action, whether in contract or tort, including negligence. Any action against National Instruments must be brought within one year after the cause of action accrues. National Instruments shall not be liable for any delay in performance due to causes beyond its reasonable control. The warranty provided herein does not cover damages, defects, malfunctions, or service failures caused by owner's failure to follow the National Instruments installation, operation, or maintenance instructions; owner's modification of the product; owner's abuse, misuse, or negligent acts; and power failure or surges, fire, flood, accident, actions of third parties, or other events outside reasonable control.

Copyright

Under the copyright laws, this publication may not be reproduced or transmitted in any form, electronic or mechanical, including photocopying, recording, storing in an information retrieval system, or translating, in whole or in part, without the prior written consent of National Instruments Corporation.

Trademarks

LabVIEW®, NI-DAQ®, and RTSI® are trademarks of National Instruments Corporation.

Product names and company names listed are trademarks or trade names of their respective companies.

Warning Regarding Medical and Clinical Use of National Instruments Products

National Instruments products are not designed with components and testing intended to ensure a level of reliability suitable for use in treatment and diagnosis of humans. Applications of National Instruments products involving medical or clinical treatment can create a potential for accidental injury caused by product failure, or by errors on the part of the user or application designer. Any use or application of National Instruments products for or involving medical or clinical treatment must be performed by properly trained and qualified medical personnel, and all traditional medical safeguards, equipment, and procedures that are appropriate in the particular situation to prevent serious injury or death should always continue to be used when National Instruments products are being used. National Instruments products are NOT intended to be a substitute for any form of established process, procedure, or equipment used to monitor or safeguard human health and safety in medical or clinical treatment.

Contents

| | |
|---|------|
| About This Manual | ix |
| Organization of This Manual | ix |
| Conventions Used in This Manual..... | x |
| The National Instruments Documentation Set..... | x |
| Related Documentation | xi |
| Customer Communication | xi |
| | |
| Chapter 1 | |
| Introduction | 1-1 |
| About the SC-2040..... | 1-1 |
| What You Need to Get Started | 1-1 |
| Software Programming Choices | 1-2 |
| LabVIEW and LabWindows Application Software | 1-2 |
| NI-DAQ Driver Software..... | 1-2 |
| Register-Level Programming..... | 1-4 |
| Optional Equipment | 1-4 |
| Unpacking..... | 1-4 |
| | |
| Chapter 2 | |
| Configuration and Installation | 2-1 |
| Board Configuration | 2-1 |
| Supplementary Configuration Information..... | 2-6 |
| Power Supply Selection | 2-6 |
| Shield Selection..... | 2-6 |
| DAQ Board Ground Isolation Selection..... | 2-6 |
| Gain Selection..... | 2-6 |
| Input Mode Selection..... | 2-7 |
| Installation..... | 2-8 |
| Power On Sequence | 2-8 |
| | |
| Chapter 3 | |
| Signal Connections | 3-1 |
| I/O Connector Pin Description..... | 3-1 |
| Signal Connection Description | 3-4 |
| Analog Signal Input | 3-7 |
| DC-Coupled Inputs | 3-7 |
| AC-Coupled Signals | 3-8 |
| Analog Input Ranges..... | 3-10 |
| Digital Signal Input..... | 3-11 |
| Monitoring Signal Outputs..... | 3-11 |
| Other Connection Considerations | 3-11 |

Chapter 4

| | |
|--------------------------------------|-----|
| Theory of Operation | 4-1 |
| Functional Overview | 4-1 |
| Analog Circuitry | 4-3 |
| Input Protection | 4-3 |
| Amplification | 4-3 |
| Track-and-Hold (T/H) Circuitry | 4-3 |
| Triggering from the DAQ Board | 4-4 |
| External Triggering | 4-5 |
| Output Connection | 4-6 |
| Power Supply | 4-6 |

Chapter 5

| | |
|-------------------------------------|-----|
| Calibration Procedures | 5-1 |
| Software Calibration | 5-1 |
| Offset Adjustment | 5-1 |
| Gain Adjustment | 5-2 |
| Linearity Adjustment | 5-2 |
| Hardware Calibration | 5-2 |

Appendix A

| | |
|-----------------------------|-----|
| Specifications | A-1 |
|-----------------------------|-----|

Appendix B

| | |
|-------------------------------------|-----|
| Customer Communication | B-1 |
|-------------------------------------|-----|

| | |
|-----------------------|------------|
| Glossary | Glossary-1 |
|-----------------------|------------|

| | |
|--------------------|---------|
| Index | Index-1 |
|--------------------|---------|

Figures

| | | |
|-------------|---|------|
| Figure 1-1. | The Relationship between the Programming Environment, NI-DAQ, and Your Hardware | 1-3 |
| Figure 2-1. | SC-2040 Parts Locator Diagram..... | 2-2 |
| Figure 3-1. | SC-2040 I/O Connectors J11 and J12..... | 3-2 |
| Figure 3-2. | SC-2040 Signal Routing..... | 3-6 |
| Figure 3-3. | Ground-Referenced Signal Connection..... | 3-7 |
| Figure 3-4. | Floating Signal Connection | 3-8 |
| Figure 3-5. | Ground-Referenced AC-Coupled Signal Connection | 3-9 |
| Figure 3-6. | Ground-Offset AC-Coupled Signal Connection..... | 3-9 |
| Figure 3-7. | Floating AC-Coupled Signal Connection..... | 3-10 |
| Figure 4-1. | SC-2040 Block Diagram..... | 4-2 |
| Figure 4-2. | T/H Amplifier Hold Settling Time and Track Acquisition Time..... | 4-4 |
| Figure 4-3. | MIO-16E Controlled Triggering..... | 4-5 |
| Figure 4-4. | External Triggering..... | 4-6 |

Tables

| | | |
|------------|---|-----|
| Table 2-1. | Power Supply Selection..... | 2-3 |
| Table 2-2. | Shield Selection | 2-4 |
| Table 2-3. | DAQ Board Ground Isolation Selection..... | 2-4 |
| Table 2-4. | Channel Gain Selection | 2-5 |
| Table 2-5. | Channel Input Mode | 2-5 |
| Table 2-6. | Gain Switches for Each Channel..... | 2-6 |
| Table 2-7. | Switch Settings for Gain Selection..... | 2-7 |
| Table 2-8. | Input Mode Selection Jumpers | 2-7 |
| Table 3-1. | Pin Assignments for Connectors J11 and J12..... | 3-3 |
| Table 3-2. | Input Connectors Signal Summary..... | 3-4 |
| Table 3-3. | Output Connectors (J11 and J12) Signal Summary..... | 3-4 |
| Table 5-1. | Calibration Component Identification..... | 5-3 |

About This Manual

This manual describes the electrical and mechanical aspects of the SC-2040 and contains information concerning its configuration and operation. The SC-2040 is an eight-channel simultaneously sampling differential amplifier for the National Instruments MIO-16E Series DAQ boards. The SC-2040 samples all eight channels at the same time, preserving interchannel phase relationships for the MIO-16E.

Organization of This Manual

The *SC-2040 User Manual* is organized as follows:

- Chapter 1, *Introduction*, describes the SC-2040, lists what you need to get started with your SC-2040, describes the optional software and optional equipment, and explains how to unpack your SC-2040.
- Chapter 2, *Configuration and Installation*, describes the configuration and installation of your SC-2040. The topics discussed are switch and jumper configuration, connection of the SC-2040 to the MIO-16E, and the power-on sequence for your SC-2040 configuration.
- Chapter 3, *Signal Connections*, describes the signal connections to the SC-2040 board, and cable wiring.
- Chapter 4, *Theory of Operation*, contains a functional overview of the SC-2040 board and explains the operation of each functional unit making up the SC-2040.
- Chapter 5, *Calibration Procedures*, discusses the calibration procedures for the SC-2040 board.
- Appendix A, *Specifications*, lists the specifications for the SC-2040.
- Appendix B, *Customer Communication*, contains forms you can use to request help from National Instruments or to comment on our products.
- The *Glossary* contains an alphabetical list and description of terms used in this manual, including abbreviations, acronyms, metric prefixes, mnemonics, and symbols.
- The *Index* contains an alphabetical list of key terms and topics used in this manual, including the page where you can find each one.

Conventions Used in This Manual

The following conventions are used in this manual:

| | |
|---------------------------|---|
| <i>bold italic</i> | Bold, italic text denotes a note, caution, or warning. |
| <i>italic</i> | Italic text denotes emphasis, a cross reference, or an introduction to a key concept. |
| MIO-16E | MIO-16E refers to the National Instruments E-Series of MIO-16 DAQ boards unless otherwise noted. |
| monospace | Lowercase text in this font denotes text or characters that are to be literally input from the keyboard, sections of code, programming examples, and syntax examples. This font is also used for the proper names of disk drives, paths, directories, programs, subprograms, subroutines, device names, functions, variables, filenames, and extensions, and for statements and comments taken from program code. |

Abbreviations, acronyms, metric prefixes, mnemonics, symbols, and terms are listed in the *Glossary*.

The National Instruments Documentation Set

The *SC-2040 User Manual* is one piece of the documentation set for your system. You could have any of several types of manuals, depending on the hardware and software in your system. Use the manuals you have as follows:

- Your DAQ hardware user manuals—These manuals have detailed information about the DAQ hardware that plugs into or is connected to your computer. Use these manuals for hardware installation and configuration instructions, specification information about your DAQ hardware, and application hints.
- Software manuals—Examples of software manuals you might have are the LabVIEW and LabWindows® manual sets and the NI-DAQ manuals. After you set up your hardware system, use either the application software (LabVIEW or LabWindows) manuals or the NI-DAQ manuals to help you write your application. If you have a large and complicated system, it is worthwhile to look through the software manuals before you configure your hardware.
- Accessory manuals—If you are using accessory products, read the terminal block and cable assembly installation guides or accessory board user manuals. They explain how to physically connect the relevant pieces of the system together. Consult these guides when you are making your connections.

Related Documentation

The following document contains information that you may find helpful as you read this manual:

- Your DAQ hardware user manual

Customer Communication

National Instruments wants to receive your comments on our products and manuals. We are interested in the applications you develop with our products, and we want to help if you have problems with them. To make it easy for you to contact us, this manual contains comment and configuration forms for you to complete. These forms are in Appendix B, *Customer Communication*, at the end of this manual.

Chapter 1

Introduction

This chapter describes the SC-2040, lists what you need to get started with your SC-2040, describes the optional software and optional equipment, and explains how to unpack your SC-2040.

About the SC-2040

The SC-2040 is an eight-channel simultaneously sampling differential amplifier for the National Instruments MIO-16E Series DAQ boards. Each channel provides DIP-switch-selectable gain followed by a track-and-hold amplifier. The track-and-hold amplifiers sample all the inputs at the same time, which is useful for preserving interchannel phase relationships. The MIO-16E can trigger the track-and-hold amplifiers, or you can supply an external trigger source.

Note: *When a board is referred to without an AT prefix (that is, MIO-16E), the reference applies to the AT versions of that board.*

The SC-2040 is a circuitboard assembly that is placed on a workbench or mounted in a 19-in. rack. You can configure the SC-2040 to draw power from the MIO-16E board or from an external +5 V supply. A red LED indicates when the board is powered on. Input signal leads are attached at screw terminals.

What You Need to Get Started

To set up and use your SC-2040, you will need the following components:

- SC-2040 board
- *SC-2040 User Manual*
- 1.0, 2.0, 5.0, or 10.0 m SH6868 or R6868 cable

Detailed specifications of the SC-2040 are in Appendix A, *Specifications*.

Software Programming Choices

Your SC-2040 kit does not include software. There are four options to choose from when programming your National Instruments DAQ and SCXI hardware. You can use LabVIEW, LabWindows, NI-DAQ, or register-level programming software.

The SC-2040 works with LabVIEW for Windows, LabVIEW for Macintosh, LabWindows for DOS, LabWindows/CVI for Windows, NI-DAQ software for PC compatibles, and NI-DAQ software for Macintosh.

LabVIEW and LabWindows Application Software

LabVIEW and LabWindows are innovative program development software packages for data acquisition and control applications. LabVIEW uses graphical programming, whereas LabWindows enhances traditional programming languages. Both packages include extensive libraries for data acquisition, instrument control, data analysis, and graphical data presentation.

LabVIEW currently runs on three different platforms—AT/MC/EISA computers running Microsoft Windows, the Macintosh platform, and the Sun SPARCstation platform. LabVIEW features interactive graphics, a state-of-the-art user interface, and a powerful graphical programming language. The LabVIEW Data Acquisition VI Library, a series of VIs for using LabVIEW with National Instruments DAQ hardware, is included with LabVIEW. The LabVIEW Data Acquisition VI Libraries are functionally equivalent to the NI-DAQ software, except that the SCXI functions are not included in the LabVIEW software for Sun.

LabWindows has two versions—LabWindows for DOS is for use on PCs running DOS, and LabWindows/CVI is for use on PCs running Windows and for Sun SPARCstations. LabWindows/CVI features interactive graphics, a state-of-the-art user interface, and uses the ANSI standard C programming language. The LabWindows Data Acquisition Library, a series of functions for using LabWindows with National Instruments DAQ hardware, is included with the NI-DAQ software kit. The LabWindows Data Acquisition libraries are functionally equivalent to the NI-DAQ software, except that the SCXI functions are not included in the LabWindows/CVI software for Sun.

Using LabVIEW or LabWindows software will greatly reduce the development time for your data acquisition and control application.

NI-DAQ Driver Software

The NI-DAQ driver software is included at no charge with all National Instruments DAQ hardware. NI-DAQ is not packaged with SCXI or accessory products. NI-DAQ has an extensive library of functions that you can call from your application programming environment. These functions include routines for analog input (A/D conversion), buffered data acquisition (high-speed A/D conversion), analog output (D/A conversion), waveform generation, digital I/O, counter/timer operations, SCXI, RTSI, self-calibration, messaging, and acquiring data to extended memory.

NI-DAQ also internally addresses many of the complex issues between the computer and the DAQ hardware such as programming interrupts and DMA controllers. NI-DAQ maintains a consistent software interface among its different versions so that you can change platforms with minimal modifications to your code. Figure 1-1 illustrates the relationship between NI-DAQ and LabVIEW and LabWindows. You can see that the data acquisition parts of LabVIEW and LabWindows are functionally equivalent to the NI-DAQ software.

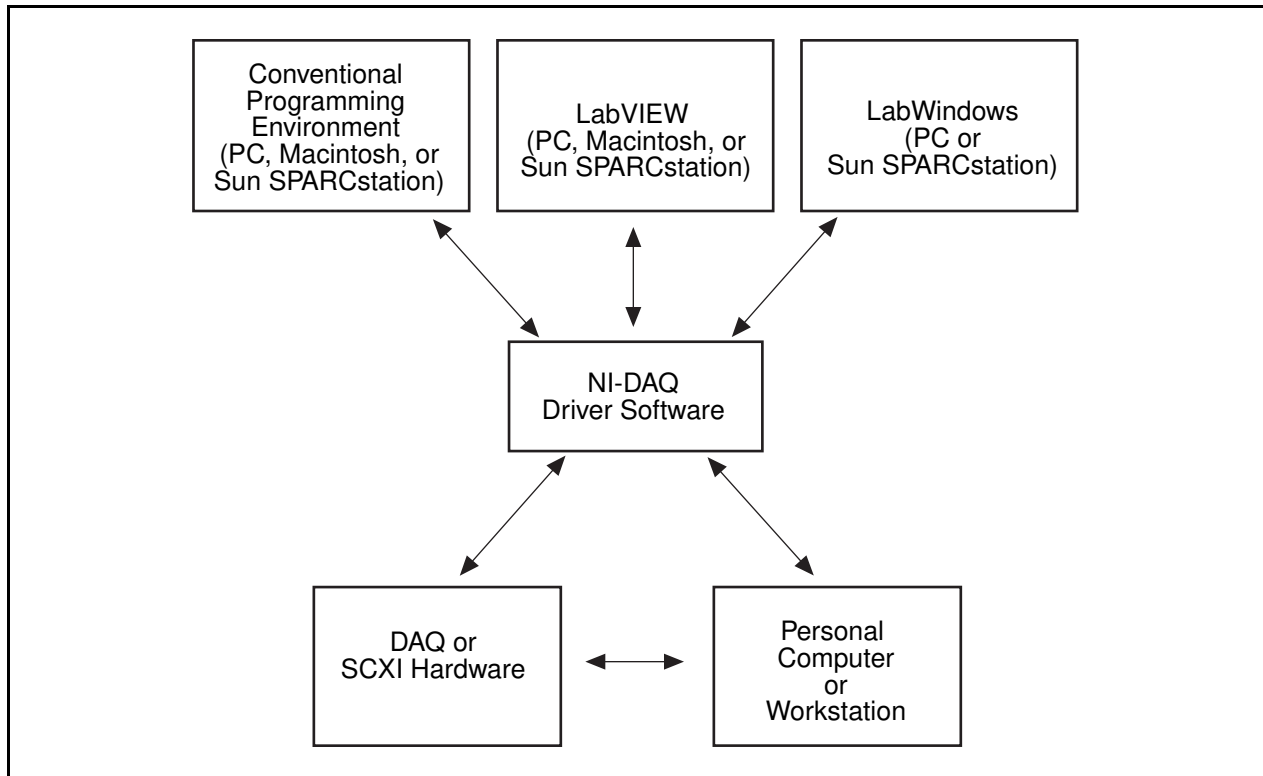


Figure 1-1. The Relationship between the Programming Environment, NI-DAQ, and Your Hardware

The National Instruments PC, AT, MC, EISA, DAQCard, and DAQPad Series DAQ hardware is packaged with NI-DAQ software for PC compatibles. NI-DAQ software for PC compatibles comes with language interfaces for Professional BASIC, Turbo Pascal, Turbo C, Turbo C++, Borland C++, and Microsoft C for DOS; and Visual Basic, Turbo Pascal, Microsoft C with SDK, and Borland C++ for Windows. You can use your AT-MIO-16, together with other PC, AT, MC, EISA, DAQCard, and DAQPad Series DAQ and SCXI hardware, with NI-DAQ software for PC compatibles.

The National Instruments NB Series DAQ boards are packaged with NI-DAQ software for Macintosh. NI-DAQ software for Macintosh comes with language interfaces for MPW C, THINK C, Pascal, and Microsoft QuickBASIC. Any language that uses Device Manager Toolbox calls can access NI-DAQ software for Macintosh. You can use NB Series DAQ boards and SCXI hardware with NI-DAQ software for Macintosh.

The National Instruments SB Series DAQ boards are packaged with NI-DAQ software for Sun, which comes with a language interface for ANSI C.

Register-Level Programming

There are no register-level programming concerns for the SC-2040. When using the SC-2040, only the MIO-16E Series board needs to be programmed. Refer to your MIO-16E board manual for further information on register-level programming.

Optional Equipment

Contact National Instruments to order the following optional equipment:

- CB-50 I/O connector (50-screw terminals) with 0.5 or 1.0 m cable
- Single or double height rack-mount kit with acrylic plastic cover
- Single or double height rack-mount kit with metal wraparound cover

Unpacking

Your SC-2040 board is shipped in an antistatic package to prevent electrostatic damage to the board. Electrostatic discharge can damage several components on the board. To avoid such damage in handling the board, take the following precautions:

- Ground yourself via a grounding strap or by holding a grounded chassis such as a computer chassis.
- Touch the antistatic package to a metal part of your computer chassis before removing the board from the package.
- Remove the board from the package and inspect the board for loose components or any other sign of damage. Notify National Instruments if the board appears damaged in any way. *Do not* install a damaged board into your computer.
- *Never* touch the exposed pins of connectors.

Chapter 2

Configuration and Installation

This chapter describes the configuration and installation of your SC-2040. The topics discussed are switch and jumper configuration, connection of the SC-2040 to the MIO-16E, and the power-on sequence for your SC-2040 configuration.

Board Configuration

The SC-2040 has 10 jumpers, eight DIP switches, and one slide switch that you use to configure the board. These switches and jumpers are shown in Figure 2-1.

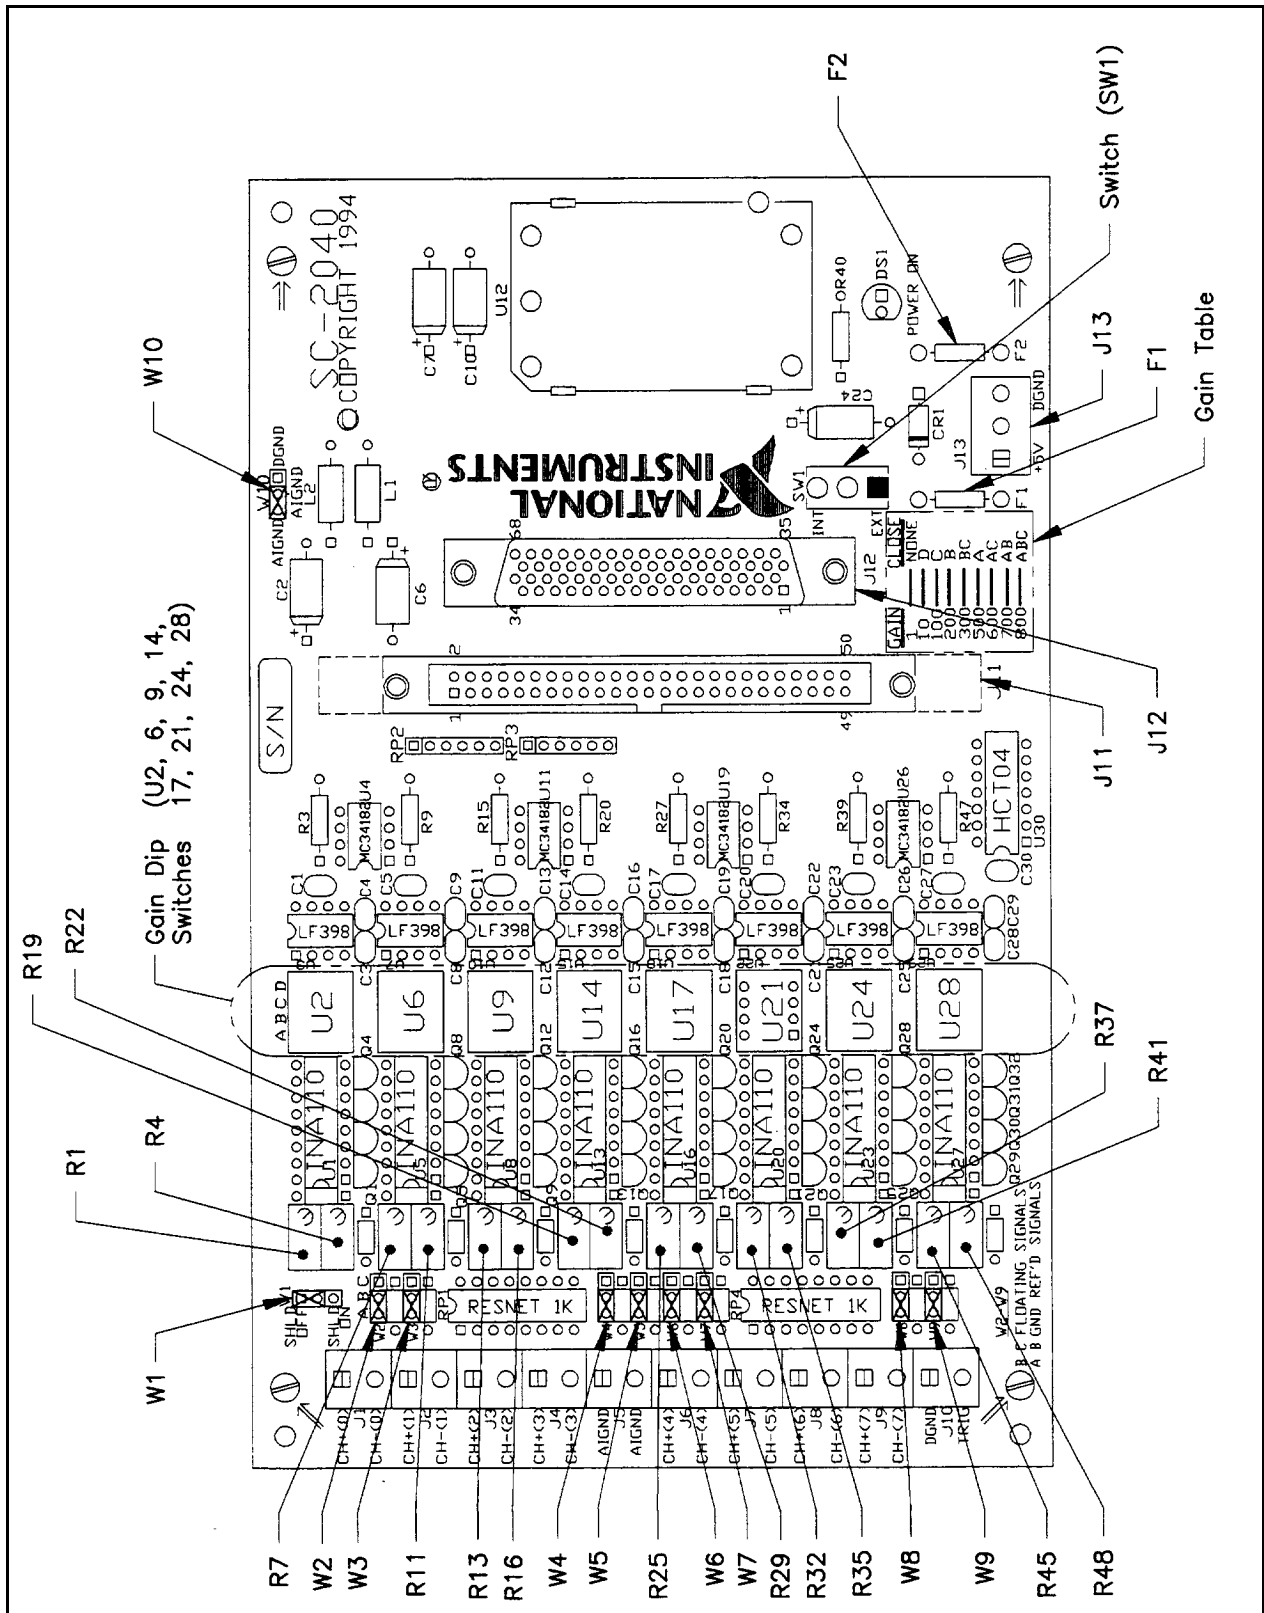


Figure 2-1. SC-2040 Parts Locator Diagram

The SC-2040 has one switch that controls whether the board is powered from an external supply or from the MIO-16E board. Furthermore, two jumpers control how the board is shielded and grounded. Additionally, there are eight sets of switches and jumpers that configure the gain settings and input modes of the eight SC-2040 channels.

Table 2-1. Power Supply Selection

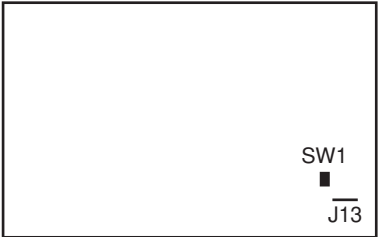


| Switch | Description | Configuration |
|---|--|--|
|  | <p>INT position—Use this setting to configure the SC-2040 to draw power through the MIO-16E board. (factory setting)</p> <p>EXT position—Use this setting to draw +5 V power from an external supply connected to connector J13.</p> | <p>SW1</p> <p>INT</p> <p>EXT</p>  <p>A. Internal Power</p> <p>SW1</p> <p>INT</p> <p>EXT</p>  <p>B. External Power</p> |

Table 2-2. Shield Selection



| Jumper | Description | Configuration |
|--|--|--|
| <div style="border: 1px solid black; padding: 5px; width: fit-content;">W1 —</div> | <p>SHLD OFF position—Place the jumper in this position to keep the SC-2040 analog ground isolated from the metal standoffs in the corners of the board (factory setting).</p> <p>SHLD ON position—Place the jumper in this position to connect the SC-2040 analog ground to the metal standoffs or to a rack-mount kit, which may provide shielding for the SC-2040.</p> | <div style="text-align: center;"> <p>W1</p>  <p>SHLD OFF</p> <p>SHLD ON</p> </div> <div style="text-align: center;"> <p>W1</p>  <p>SHLD OFF</p> <p>SHLD ON</p> </div> |

Table 2-3. DAQ Board Ground Isolation Selection



| Jumper | Description | Configuration |
|--|---|--|
| <div style="border: 1px solid black; padding: 5px; width: fit-content; text-align: right;">W10 —</div> | <p>AIGND-AIGND position—Use this setting if you are using a MIO-16E DAQ board. Place the jumper in this position to keep the SC-2040 digital ground and analog grounds isolated (factory setting).</p> <p>AIGND-DGND position—Place the jumper in this position to connect the SC-2040 analog ground to digital ground.</p> | <div style="text-align: center;"> <p>W10</p>  <p>AIGND</p> <p>AIGND</p> </div> <div style="text-align: center;"> <p>W10</p>  <p>AIGND</p> <p>AIGND</p> </div> |

Table 2-4. Channel Gain Selection

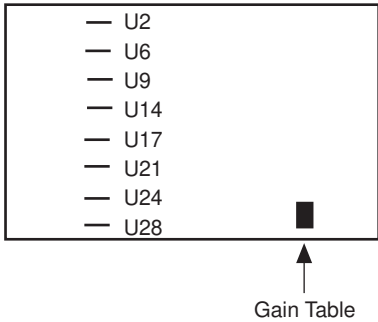




| Switch | Description | Configuration |
|---|--|--|
|  | <p>Unity gain position—For unity gain (gain = 1), open all the switches by pushing down the OFF end of the switches. (factory setting)</p> <p>Other gains—Refer to <i>Supplementary Configuration Information</i>, later in the chapter, and the gain table on the board itself.</p> |  <p>The unity gain position has the number side up.</p> |

Table 2-5. Channel Input Mode

| Switch | Description | Configuration |
|---|--|---|
|  | <p>A-B position—Use this setting for connecting ground-referenced signals to the SC-2040 (factory setting).</p> <p>B-C position—Use this setting for connecting floating (non-ground referenced) sources. A 100 kΩ resistor is connected from the negative channel input to the SC-2040 analog ground.</p> |   <p>The W3–W9 jumper positions are the same as on W2.</p> |

Supplementary Configuration Information

Power Supply Selection

Set switch SW1 to the INT position to connect the SC-2040 power converter to the +5 V lines on the MIO-16E board. Set switch SW1 to the EXT position to draw power from an external +5 V power supply connected to J13.

The MIO-16E is fused to provide 5 W of power (at +5 V and 1 A). The SC-2040 consumes nearly all of this available power. Therefore, if you have other DAQ accessories that you would like to power from the MIO, you should switch the SC-2040 to external power and provide an external +5 V power source. In external power mode, the SC-2040 is fuse limited to 1 A at +5 V.

Shield Selection

If you are using a rack-mount kit, shield the SC-2040 from unwanted noise by connecting the analog ground on the board to the metal chassis of the rack using jumper W1. When you set W1 to the SHLD ON position, the jumper connects the analog ground to the metal standoffs used to mount the board in a rack. In the SHLD OFF position, the SC-2040 analog ground is isolated from the metal standoffs.

DAQ Board Ground Isolation Selection

You can use jumper W10 to connect the SC-2040 digital and analog grounds. If you are using a MIO-16E board, you must isolate the grounds by leaving the jumper in its default position.

Gain Selection

The gain selection switches can select gains of 1, 10, 100, 200, 300, 500, 600, 700, and 800 for each channel, as shown in Table 2-6.

Table 2-6. Gain Switches for Each Channel

| Channel | Close Switches |
|---------|----------------|
| 0 | U2 |
| 1 | U6 |
| 2 | U9 |
| 3 | U14 |
| 4 | U17 |
| 5 | U21 |
| 6 | U24 |
| 7 | U28 |

To close a switch, push down the number side. Closing switch A selects a gain of 500. Closing switch B selects a gain of 200. Closing switch C selects a gain of 100. Closing switch D selects a gain of 10. Opening all the switches selects a gain of 1. You can select other gains by closing more than one switch, as shown in Table 2-7.

Table 2-7. Switch Settings for Gain Selection

| Desired Gain | Close Switches |
|--------------|----------------|
| 1 | None |
| 10 | D |
| 100 | C |
| 200 | B |
| 300 | B and C |
| 500 | A |
| 600 | A and C |
| 700 | A and B |
| 800 | A, B, and C |

Input Mode Selection

Jumpers W2 through W9 select the input mode for each channel on the SC-2040. Position A-B leaves the negative input of the instrumentation amplifier connected only to the front connector. This is the factory-default setting. Position B-C connects the negative input of the instrumentation amplifier to the board analog ground through a 100 k Ω resistor. This setting is useful for keeping floating, or nonground-referenced, sources from saturating the instrumentation amplifier. Table 2-8 shows the input mode jumper and channel selections.

Table 2-8. Input Mode Selection Jumpers

| Channel | Use Jumper |
|---------|------------|
| 0 | W2 |
| 1 | W3 |
| 2 | W4 |
| 3 | W5 |
| 4 | W6 |
| 5 | W7 |
| 6 | W8 |
| 7 | W9 |

Installation

Note: *You must turn off power to the PC, and to the SC-2040 board if the board is externally powered, before installing the board or making any connections to it.*

To install the SC-2040, connect the 68-pin ribbon from the MIO-16E I/O connector to connector J12 on the SC-2040. The SC-2040 can be mounted in a rack-mount chassis using the mounting holes (indicated with an arrow on the board) in the four corners of the SC-2040 board.

The SC-2040 is installed. You are now ready to install and configure your software.

If you are using NI-DAQ, refer to your NI-DAQ manual. The software installation and configuration instructions are in Chapter 1, Introduction to NI-DAQ. Find the installation and system configuration section for your operating system and follow the instructions given there.

If you are using LabVIEW, the software installation instructions are in your LabVIEW release notes. After you have installed LabVIEW, refer to the Configuring LabVIEW section of Chapter 1 of your LabVIEW user manual for software configuration instructions.

If you are using LabWindows, the software installation instructions are in Part 1, Introduction to LabWindows, of the Getting Started with LabWindows manual. After you have installed LabWindows, refer to Chapter 1, Configuring LabWindows, of the LabWindows User Manual for software configuration instructions.

Power-on Sequence

If the SC-2040 is powered by an external power source, you must turn on power to the SC-2040 *before* turning on the computer. Similarly, you must turn off power to the SC-2040 *after* turning off the computer. The red LED labeled DS1 indicates when power is applied to the board.

Chapter 3

Signal Connections

This chapter describes the signal connections to the SC-2040 board, and cable wiring.

I/O Connector Pin Description

Warning: *Connections that exceed any of the maximum ratings of input or output signals on the MIO-16 can result in damage to the MIO-16 board and to the personal computer. This includes connecting any power signals to ground and vice versa. National Instruments is not liable for any damages resulting from any such signal connections.*

Corresponding signals on connectors J11 and J12 are connected together through the SC-2040. Connector J12 carries the signals to and from the MIO-16E board. Use connector J11 to access these signals. You can use this connector to monitor these signals, using a National Instruments CB-50, for example, or you can use this connector to connect to other DAQ accessories. Figure 3-1 shows these connectors.

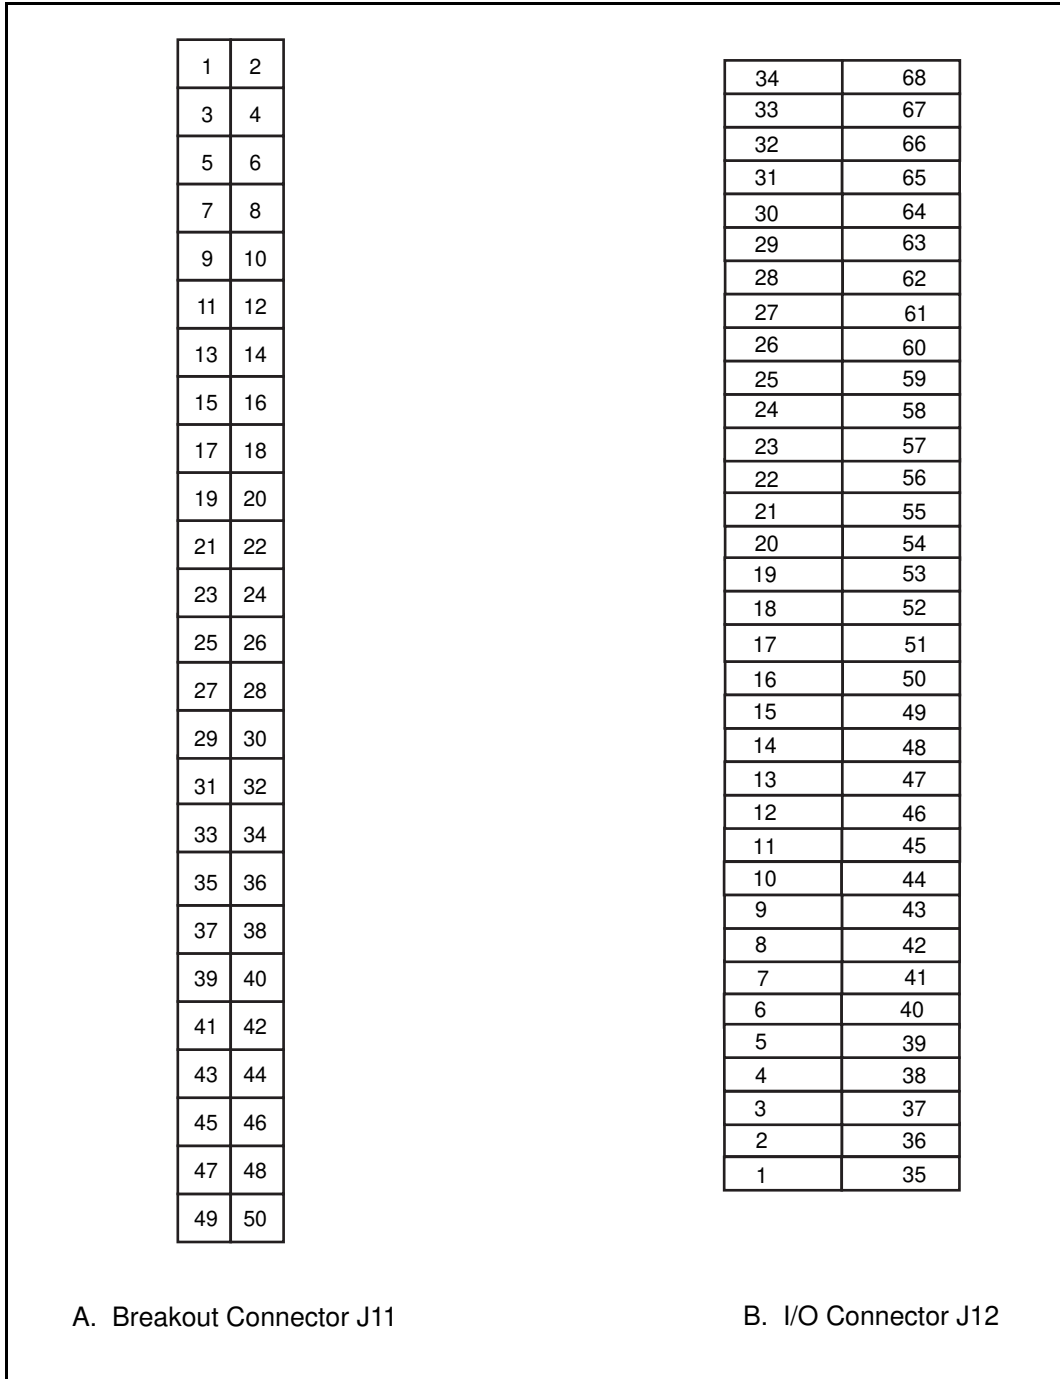


Figure 3-1. SC-2040 I/O Connectors J11 and J12

Table 3-1 lists the pin assignments for the breakout connector J11 and the I/O connector J12 on the SC-2040 and the corresponding and MIO-16E Series signal names.

Table 3-1. Pin Assignments for Connectors J11 and J12

| Breakout Connector J11 Pin Numbers | SC-2040 Signal Names ¹ | MIO-16E Series Signal Names | I/O Connector J12 Pin Numbers |
|---------------------------------------|--------------------------------------|--------------------------------|--|
| 1, 2 | AIGND | AIGND | 24, 27, 29, 32, 56, 59, 64, 67 |
| 3 | ACH0 | ACH0 | 68 |
| 4 | AIGND | ACH8 | 34 |
| 5 | ACH1 | ACH1 | 33 |
| 6 | AIGND | ACH9 | 66 |
| 7 | ACH2 | ACH2 | 65 |
| 8 | AIGND | ACH10 | 31 |
| 9 | ACH3 | ACH3 | 30 |
| 10 | AIGND | ACH11 | 63 |
| 11 | ACH4 | ACH4 | 28 |
| 12 | AIGND | ACH12 | 61 |
| 13 | ACH5 | ACH5 | 60 |
| 14 | AIGND | ACH13 | 26 |
| 15 | ACH6 | ACH6 | 25 |
| 16 | AIGND | ACH14 | 58 |
| 17 | ACH7 | ACH7 | 57 |
| 18 | AIGND | ACH15 | 23 |
| 19 | NC | AISENSE | 62 |
| 20 | NC | DAC0OUT | 22 |
| 21 | NC | DAC1OUT | 21 |
| 22 | NC | EXTREF | 20 |
| 23 | NC | AOGND | 54, 55 |
| 24, 33 | DGND | DGND | 4, 7, 9, 12, 13, 15, 18, 35, 36, 39, 44, 50, 53 |
| 25 | NC | DIO0 | 52 |
| 26 | NC | DIO4 | 19 |
| 27 | NC | DIO1 | 17 |
| 28 | NC | DIO5 | 51 |
| 29 | NC | DIO2 | 49 |
| 30 | NC | DIO6 | 16 |
| 31 | NC | DIO3 | 47 |
| 32 | NC | DIO7 | 48 |
| 34, 35 | +5V | +5V | 8, 14 |
| 36 | NC | SCANCLK | 46 |
| 37 | NC | EXTSTROBE* | 45 |
| 38 | NC | PFI0/TRIG1 | 11 |
| 39 | NC | PFI1/TRIG2 | 10 |
| 40 | TRIG | PFI2/CONVERT* | 43 |
| 41 | NC | PFI3/GPCTR1_SOURCE | 42 |
| 42 | NC | PFI4/GPCTR1_GATE | 41 |
| 43 | NC | GPCTR1_OUT | 40 |
| 44 | NC | PFI5/UPDATE* | 6 |
| 45 | NC | PFI6/WFTRIG | 5 |
| 46 | TRACK*/HOLD | PFI7/STARTSCAN | 38 |
| 47 | NC | PFI8/GPCTR0_SOURCE | 37 |
| 48 | NC | PFI9/GPCTR0_GATE | 3 |
| 49 | NC | GPCTR0_OUT | 2 |
| 50 | NC | FREQ_OUT | 1 |

¹ All signals labeled NC are unused by the SC-2040.

Signal Connection Description

Table 3-2. Input Connectors Signal Summary

| Connector | Signal Name | Description |
|--------------------------------|-------------|--|
| J5 | AIGND | Analog Input Ground—These inputs provide a bias current return point for AC-coupled signals. |
| J1, J2, J3, J4, J6, J7, J8, J9 | CH+<0..7> | Positive Inputs—These inputs are the positive signal inputs for channels 0 through 7. |
| J1, J2, J3, J4, J6, J7, J8, J9 | CH-<0..7> | Negative Inputs—These inputs are the negative signal inputs for channels 0 through 7. |
| J10, J13 | DGND | Digital Ground—These inputs provide the reference for all digital signals and the reference for the +5 V power source. |
| J10 | TRIG | Trigger—This input, which is connected directly to the PFI2 pin on connectors J11 and J12, is a triggered input for the MIO-16E. A low-to-high transition on TRIG alerts the MIO-16E to place the SC-2040 into hold mode and start acquiring data. |
| J13 | +5 V | +5 VDC Source—When external power is selected, this input provides DC power for the SC-2040 from an external +5 V. The SC-2040 fuses the input to 1 A of the +5 V supply. |

Table 3-3. Output Connectors (J11 and J12) Signal Summary

| J11 Pin (50-pin) | J12 Pin (68-pin) | Signal Name | Description |
|-----------------------------------|--|-------------|---|
| 1, 2, 4, 6, 8, 10, 12, 14, 16, 18 | 23, 24, 26, 27, 29, 31, 32, 34, 56, 58, 59, 61, 63, 64, 66, 67 | AIGND | Analog Input Ground—These pins establish the reference point for the SC-2040 outputs (ACH<0..7>). They are also connected directly to the AIGND input connector J5 for use with AC-coupled signals. |
| 3, 5, 7, 9, 11, 13, 15, 17 | 68, 33, 65, 30, 28, 60, 25, 57 | ACH<0..7> | Analog Channels 0 through 7—These pins carry the outputs of the SC-2040 eight channels to the DAQ board. They are referenced to AIGND. |
| 24, 33 | 4, 7, 9, 12, 13, 15, 18, 35, 36, 39, 44, 50, 53 | DGND | Digital Ground—These pins are the reference for the +5 V power source and for the digital signals used by the SC-2040: TRIG (PFI2) and TRACK*/HOLD (PFI7/STARTSCAN). |
| 34, 35 | 8, 14 | +5 V | +5 VDC Source—When internal power is selected, these pins provide DC power for the SC-2040 from the MIO-16E board. The MIO-16E pins are fused to 1 A of +5 V supply. |
| 40 | 43 | TRIG (PFI2) | Trigger—This pin, which is connected directly to the TRIG input on screw terminal connector J10, is a trigger input to the MIO-16E PFI2 line. A low-to-high transition on PFI2 alerts the MIO-16E to place the SC-2040 into hold mode and start acquiring data. |

(continues)

Table 3-3. Output Connectors (J11 and J12) Signal Summary (Continued)

| J11 Pin (50-pin) | J12 Pin (68-pin) | Signal Name | Description |
|---------------------|---------------------|---------------------------------|--|
| 46 | 38 | TRACK*/HOLD (PFI7/STARTSCAN) | Track-or-hold—This pin, used as an output from the MIO-16E, controls whether the SC-2040 is in hold mode or track mode. A high level output from the DAQ board places the SC-2040 into hold mode, while a low level returns the SC-2040 into track mode. <i>With an MIO-16E attached, pin 46 on J11 should be used for monitoring purposes only.</i> |
| others | others | compatibility | The remaining pins provide 50 pin compatibility with the 68 pin MIO-16E. They can be monitored from connector J11. Refer to Figure 3-1 for pin locations and to Chapter 3, <i>Signal Connections</i> , in your MIO-16E manual for pin descriptions. |

The signals from the SC-2040 screw terminal connectors are connected to the MIO-16E via J12 as shown in Figure 3-2. Observe that the PFI7/STARTSCAN signal returns from the MIO-16E as a level-sensitive track-and-hold signal to the SC-2040. Notice also that AISENSE is disconnected.

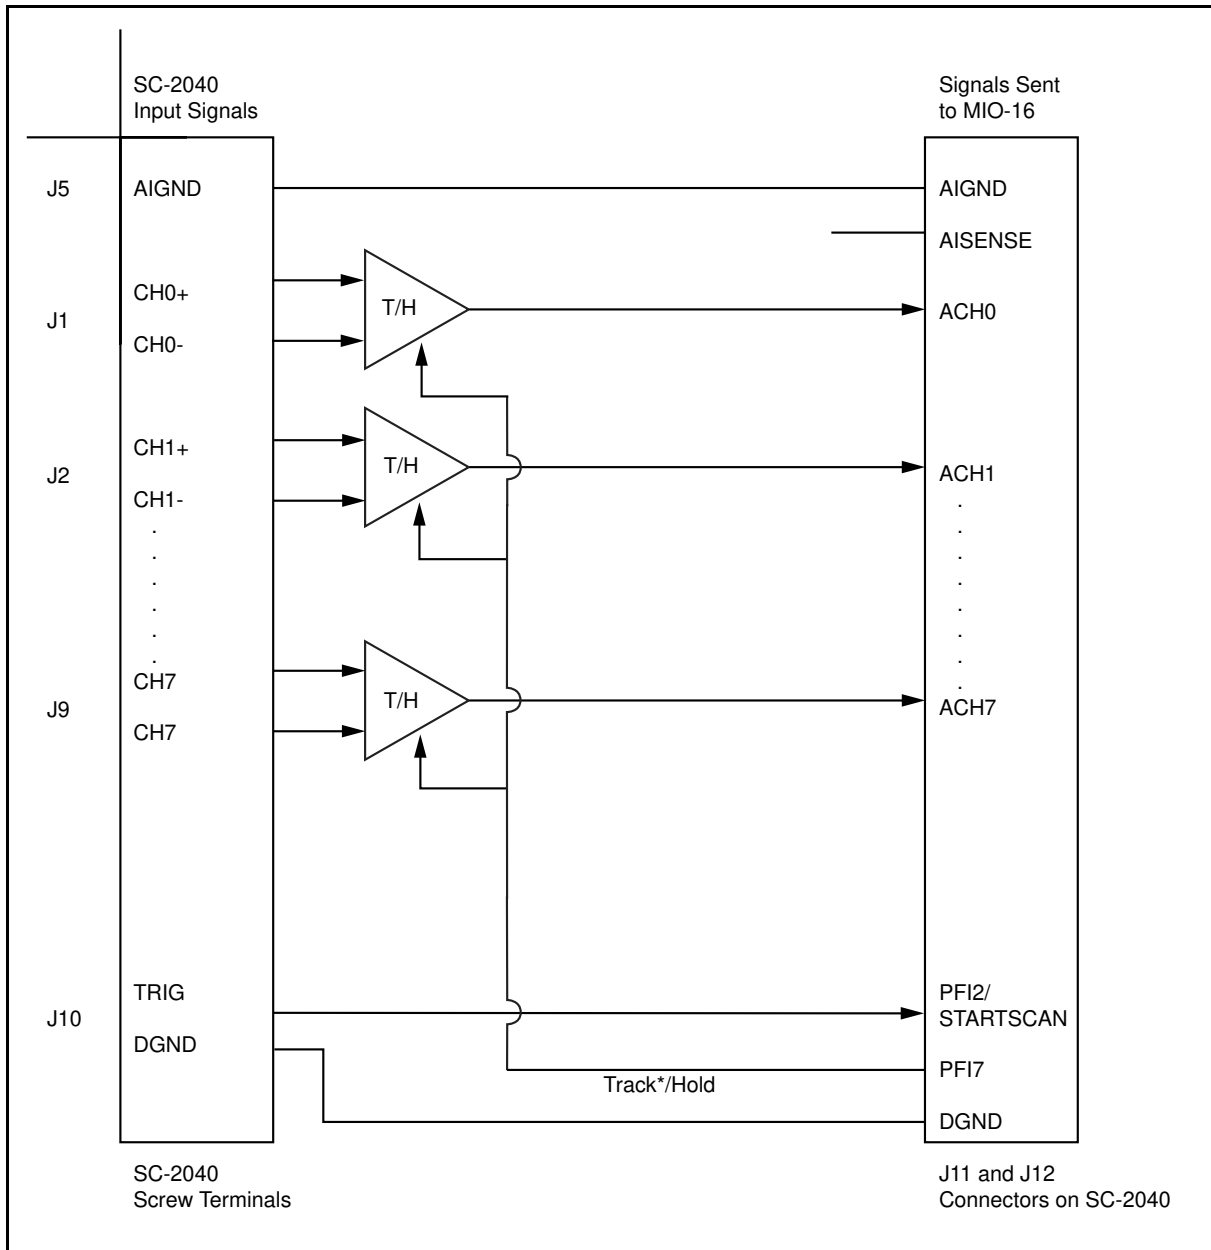


Figure 3-2. SC-2040 Signal Routing

Analog Signal Inputs

Connect the differential signals to be measured to the screw terminal connectors J1 through J4 and J5 through J9.

DC-Coupled Inputs

Note: *If all your inputs are DC-coupled, leave connector J5 disconnected.*

All eight channels have fully differential inputs, so the signals you are measuring should be ground referenced. If they are not, set jumpers W2 through W9 of the nonreferenced channels to position B-C to create a DC path for the input bias currents. If you do not do this, the bias currents of the instrumentation amplifiers of the nonreferenced channels produce stray capacitances, resulting in uncontrollable drift and possible saturation.

Figure 3-3 illustrates how to connect a ground-referenced signal.

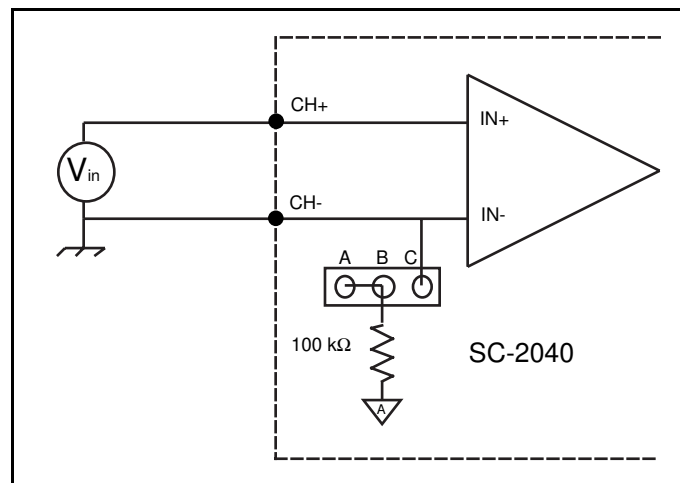


Figure 3-3. Ground-Referenced Signal Connection

Figure 3-4 illustrates how to connect a floating signal.

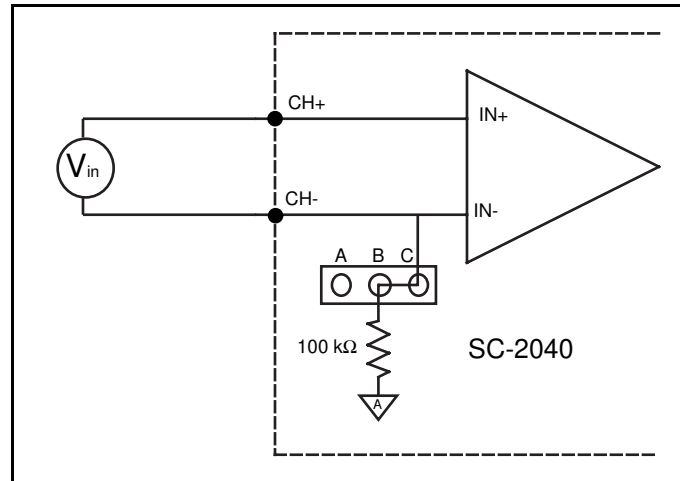


Figure 3-4. Floating Signal Connection

AC-Coupled Signals

Note: *For AC-coupled signals, you must reference the analog ground of your instrumentation to the DAQ board. The SC-2040 connector J5 provides the analog reference, connecting directly to the MIO-16E board as shown in Figure 3-2.*

For AC-coupled signals, set jumpers W2 through W9 to position B-C with an external resistor from the positive input channel connected to its negative ground. Doing this creates the DC path for the positive input bias current. Typical resistor values range from 100 kΩ to 10 MΩ. This solution, although necessary in this case, lowers the input impedance of the channel and introduces an additional offset voltage proportional to the product of the input bias current and the resistor value used. The inputs of the SC-2040 have a typical bias current of about ± 100 pA. When you use a 1 MΩ resistor, the result is ± 100 μV of offset, which is insignificant in most applications. However, if you use larger valued bias resistors, significant input offset may result. Lower valued bias resistors will increase loading of the source, possibly resulting in gain error.

Figures 3-5 through 3-7 illustrate how to connect AC-coupled signals.

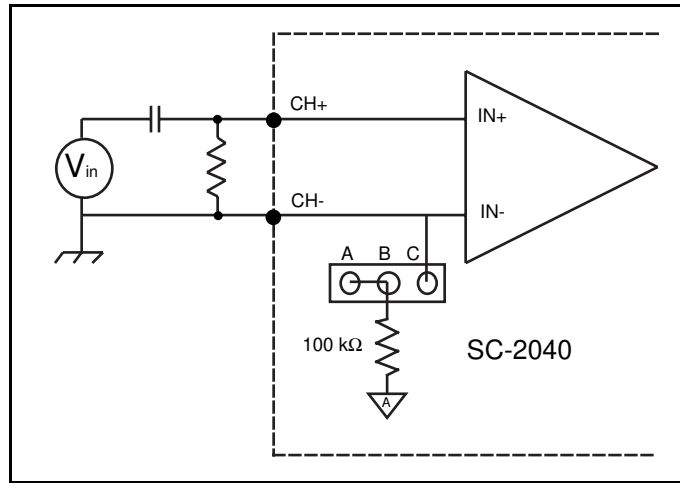


Figure 3-5. Ground-Referenced AC-Coupled Signal Connection

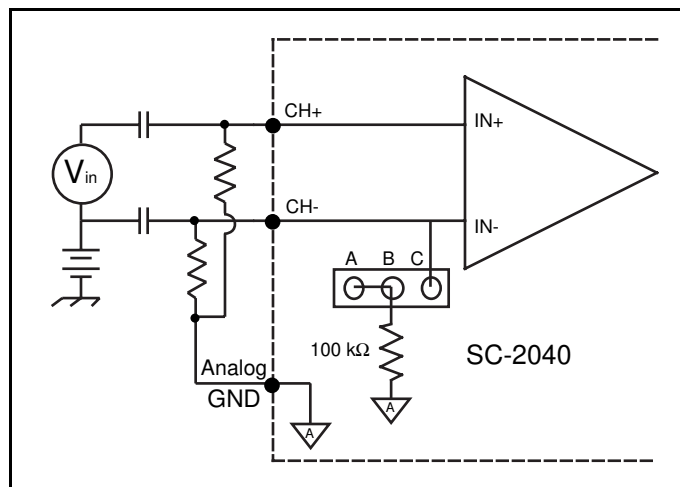


Figure 3-6. Ground-Offset AC-Coupled Signal Connection

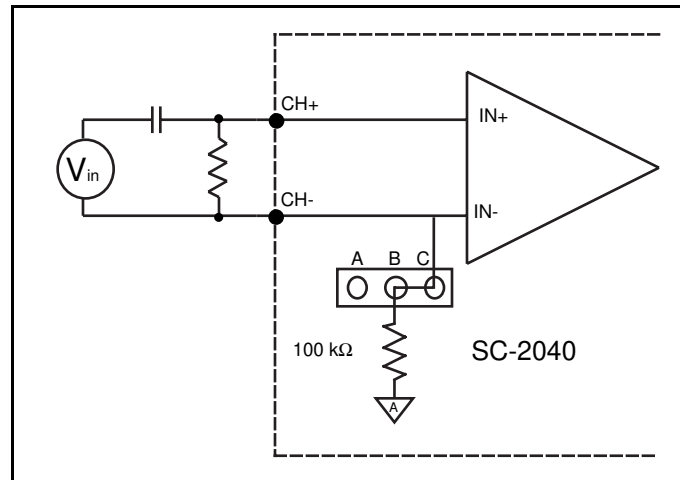


Figure 3-7. Floating AC-Coupled Signal Connection

Analog Input Ranges

Warning: *Exceeding the differential and common-mode input ranges results in distorted input signals. Exceeding the maximum input voltage rating can result in damage to the SC-2040 board, and the DAQ board. National Instruments is NOT liable for any damages resulting from such signal connections.*

The SC-2040 instrumentation amplifiers can reject any voltage within their common-mode input range caused by ground-potential differences between the signal source and the board. In addition, the amplifiers can reject common-mode noise pickup in the leads connecting the signal sources to the SC-2040 board. However, you should be careful to minimize noise pickup. The common-mode rejection of the instrumentation amplifiers decreases significantly at high frequencies. The amplifiers do not reject normal-mode noise.

The common-mode input range of the SC-2040 instrumentation amplifiers is defined as the magnitude of the greatest common-mode signal that can be rejected. Thus the common-mode input range for the SC-2040 depends on the gain and size of the differential input signal:

$$(V_{diff} = V_{in}^{+} - V_{in}^{-}).$$

The exact formula for the permissible common-mode input range is as follows:

$$V_{cm-allowed} = \pm \left(12 \text{ V} - \frac{G |V_{diff}|}{2} \right).$$

Thus, with a differential voltage of 10 V and a gain of $G = 1$, the maximum possible common-mode voltage would be ± 7 V. The same range would apply for a differential input of 100 mV and a gain of 100. The range increases to ± 12 V for zero differential input voltage. The actual common-mode voltage available at the input is measured with respect to the SC-2040 ground, and can be calculated by the following formula:

$$V_{cm-actual} = \frac{(V_{in}^{+} - V_{in}^{-})}{2}.$$

where V_{in}^+ is the signal at the positive input (IN0+ through IN7+), and V_{in}^- is the signal at the corresponding negative input (IN0- through IN7-). Both V_{in}^+ and V_{in}^- are measured with respect to the SC-2040 chassis ground.

Digital Signal Inputs

If you are using an external trigger, connect the trigger source and the digital reference to screw connector J9. This signal should be in the range 0 to +5 V, with switching occurring around 1.5 V.

Note: *All digital signals on the SC-2040 are referenced to the +5 V power supply. If the MIO-16E supplies power, it provides this reference. If an external supply provides power, it provides this reference through connector J13.*

A rising edge on the trigger will place the SC-2040 into hold mode, and the SC-2040 will return to track mode when the MIO-16E indicates that the data acquisition is complete.

Although the TRIG signal is a digital signal, it is still susceptible to noise, particularly at its transitions. This noise can cause the SC-2040 to enter hold mode on the wrong edge. Two possible sources of noise are interference and reflection. The best way to reduce noise corruption is to minimize the distance that the signal must travel. Furthermore, you can minimize interference by properly shielding the incoming trigger signal. You can minimize reflection by ensuring that the impedance of the source of the trigger signal matches the impedance of the cable used to transmit the signal; inserting a small resistor (about 50 Ω) in series with the signal source will minimize reflection.

Monitoring Signal Outputs

You can use connector J11 to monitor the signals being sent to and from the MIO-16E board. Figure 4-3 shows a sampled analog signal as the SC-2040 channel output.

You can also monitor the state of the SC-2040 through line PFI7/STARTSCAN. A high level on PFI7/STARTSCAN indicates the SC-2040 is in hold mode, while a low level indicates that the SC-2040 is in track mode.

Other Connection Considerations

Refer to the sections titled *Analog Input Signal Connections* and *Cabling and Field Wiring* in Chapter 3 of your MIO-16E board user manual for additional signal connection information.

Chapter 4

Theory of Operation

This chapter contains a functional overview of the SC-2040 board and explains the operation of each functional unit making up the SC-2040.

Functional Overview

The SC-2040 consists of eight channels, each one comprising an instrumentation amplifier with DIP switch-programmable gains of 1, 10, 100, 200, 300, 500, 600, 700, or 800, and a track-and-hold amplifier. The analog inputs are overvoltage protected. The DAQ board or a user-supplied external trigger switches the SC-2040 between hold mode and track mode as desired. All eight channels are simultaneously placed in hold mode.

The block diagram in Figure 4-1 illustrates the key functional components of the SC-2040.

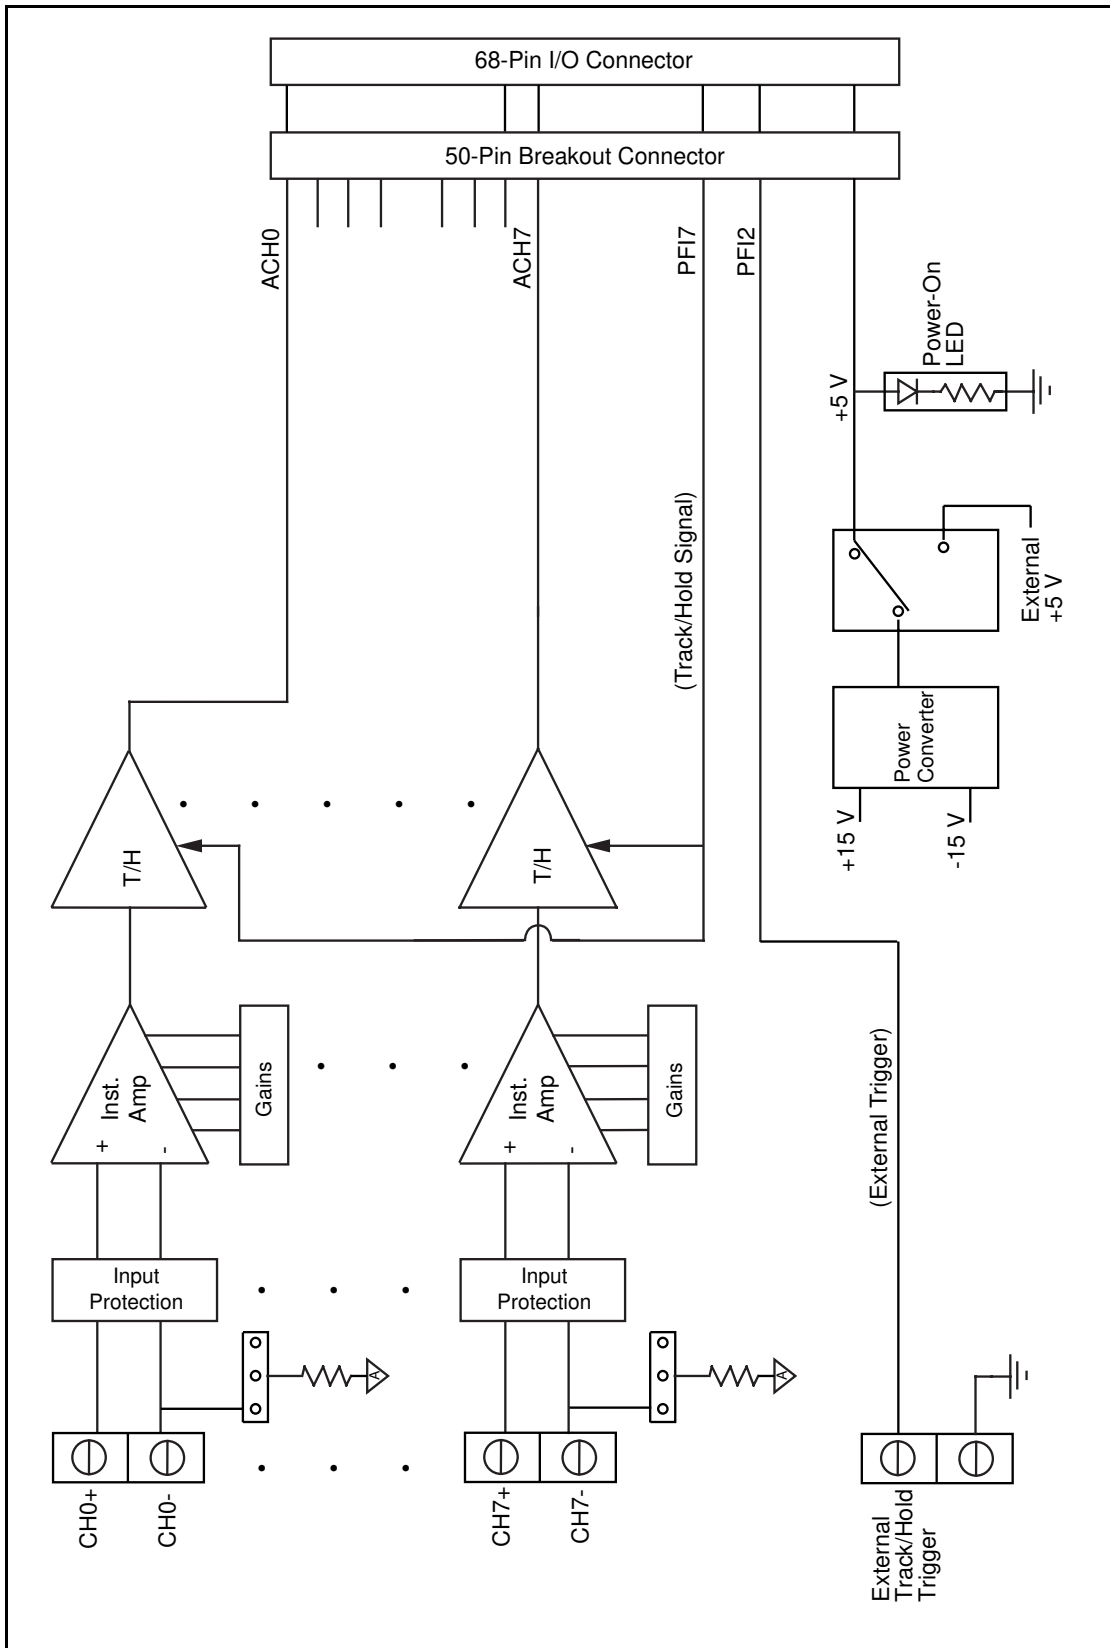


Figure 4-1. SC-2040 Block Diagram

Analog Circuitry

The analog input circuitry consists of eight channels with DIP-switch-programmable instrumentation amplifiers followed by buffered track-and-hold amplifiers. In addition, you can include the voltage-regulation circuitry and input protection in the analog section. Each block is described in the following paragraphs.

Input Protection

The first block an incoming analog signal encounters is the input protection. Each input terminal is protected against input voltages up to ± 15 V powered off and ± 30 V powered on. The input protection consists of a 1 k Ω resistor in series with each input line followed by low-leakage diodes to the supply rails (± 15 V).

Amplification

Next in the signal path are the instrumentation amplifiers, which fulfill two purposes on the SC-2040 board. First, the instrumentation amplifiers convert differential input signals into single-ended signals referred to the SC-2040 analog ground for input common-mode signal rejection. With this conversion, the SC-2040 can extract the analog input signals from common-mode noise voltages before the DAQ board samples and converts the signals. Second, the instrumentation amplifiers amplify input signals, resulting in an increase in measurement resolution and accuracy. Furthermore, the amplifiers exhibit low bias currents and good bandwidth, even at high gains.

You can select gains for each channel independently with separate DIP switches. Gains are 1, 10, 100, 200, and 500, although gains of 300, 600, 700, and 800 are available with reduced accuracy. See Appendix A, *Specifications*, for details on the performance of the instrumentation amplifiers.

Track-and-Hold (T/H) Circuitry

The track-and-hold amplifiers operate as simple buffers when in track mode, but freeze their outputs when placed into hold mode. Because all of the track-and-hold amplifiers in each SC-2040 board enter hold mode at the same time, they implement simultaneous sampling of all channels. Simultaneous sampling is useful for preserving phase relationships between channels.

The track-and-hold amplifiers are subject to various imperfections, which are listed in Appendix A, *Specifications*. The most relevant of these performance specifications are the track-mode acquisition time and the hold-mode settling time, as these parameters affect how the DAQ board acquires the data, most noticeably through the sampling rate.

The hold-mode settling time refers to how long it takes the T/H amplifiers to settle a stable value. Thus, the hold-mode settling time affects how long the DAQ board must wait *before* attempting to acquire data. The track-mode acquisition time refers to how long it takes the T/H amplifiers to

find the inputs again after having been in hold mode. Therefore, this delay indicates how long the SC-2040 must remain in track mode before it is ready to re-enter hold mode. Returning the SC-2040 to hold mode before the track-mode acquisition delay has elapsed will cause the SC-2040 to "hold" erroneously. Figure 4-2 illustrates these timing concerns. Typical hold mode settling times and track acquisition times for 12-bit and 16-bit accuracies are given in Appendix A, *Specifications*.

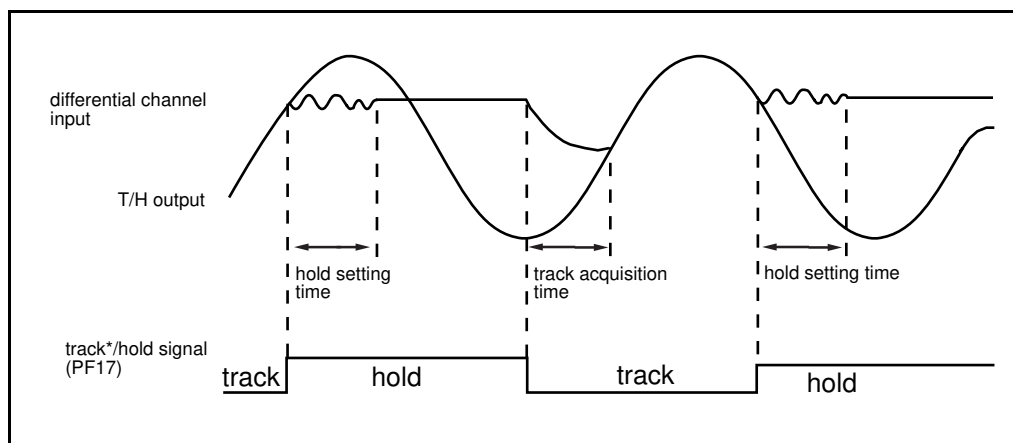


Figure 4-2. T/H Amplifier Hold Settling Time and Track Acquisition Time

Triggering from the DAQ Board

This section applies to you only if you are triggering the SC-2040 from the MIO-16E board.

Note: *No signal should be connected to connector J10 for MIO-16E triggering.*

You can place the SC-2040 into hold mode on command using the MIO-16E DAQ board. You must either program the MIO-16E board for this purpose or use the NI-DAQ software included with your MIO board. After placing the SC-2040 into hold mode, the MIO-16E board performs data acquisition and conversion. Once this process is complete, the MIO-16E board releases the SC-2040 into track mode.

The MIO-16E board uses line PFI7/STARTSCAN to indicate to the SC-2040 whether it should track the input signals or hold them at a constant level. A logic zero (low level) on PFI7/STARTSCAN indicates track mode, while a logic one (high level) indicates hold mode, as indicated in Figure 4-3.

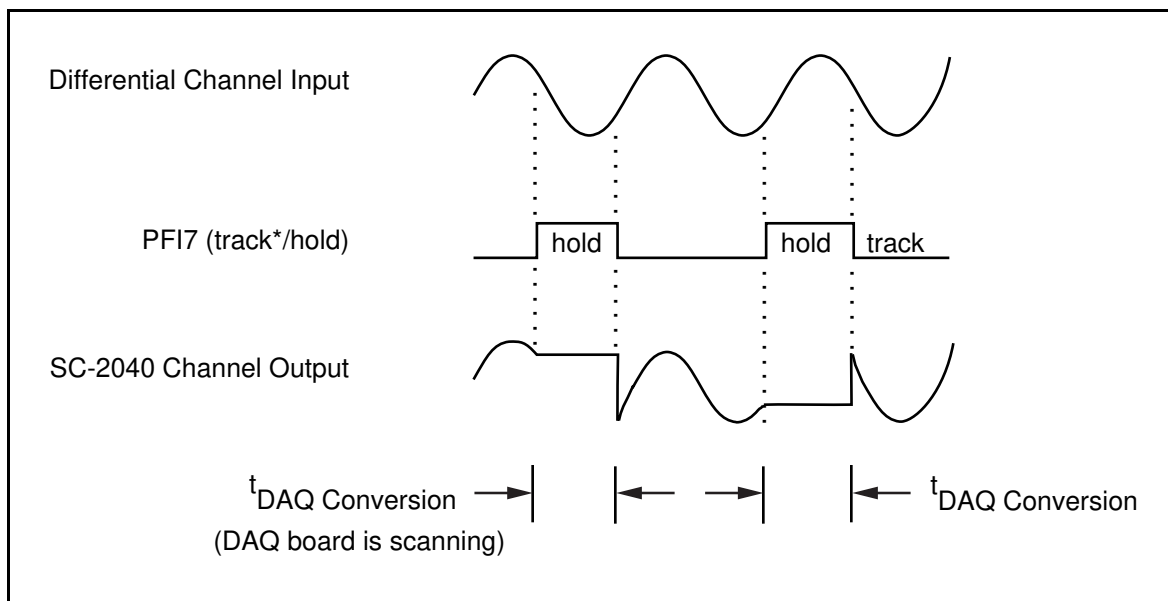


Figure 4-3. MIO-16E Controlled Triggering

External Triggering

This section applies to you only if you are triggering the board from an external signal connected to J10.

You can connect an external trigger to place the SC-2040 into hold mode on command. A rising edge on the external trigger signal places the SC-2040 into hold mode and alerts the MIO-16E board to start scanning the SC-2040 outputs. After the MIO-16E board has acquired data from all of the channels, it returns the SC-2040 to track mode. The external trigger signal is a digital input and must conform to digital logic levels.

Because the SC-2040 track-and-hold circuitry must re-acquire the input signals at the conclusion of each hold mode operation, the external trigger source should not return the SC-2040 to hold mode until after the SC-2040 has had time to re-acquire the signals. The acquisition times for the SC-2040 at various accuracies are given in Appendix A, *Specifications*.

The external trigger is connected directly to signal PFI2 on the DAQ board. A rising edge alerts the DAQ board to place the SC-2040 into hold mode. The DAQ board then begins scanning the channels. After the scanning process is complete, the board returns the SC-2040 to track mode using PFI7/STARTSCAN. Notice that additional rising edges from the external trigger are ignored while the MIO-16E is scanning. Figure 4-4 illustrates the external triggering process.

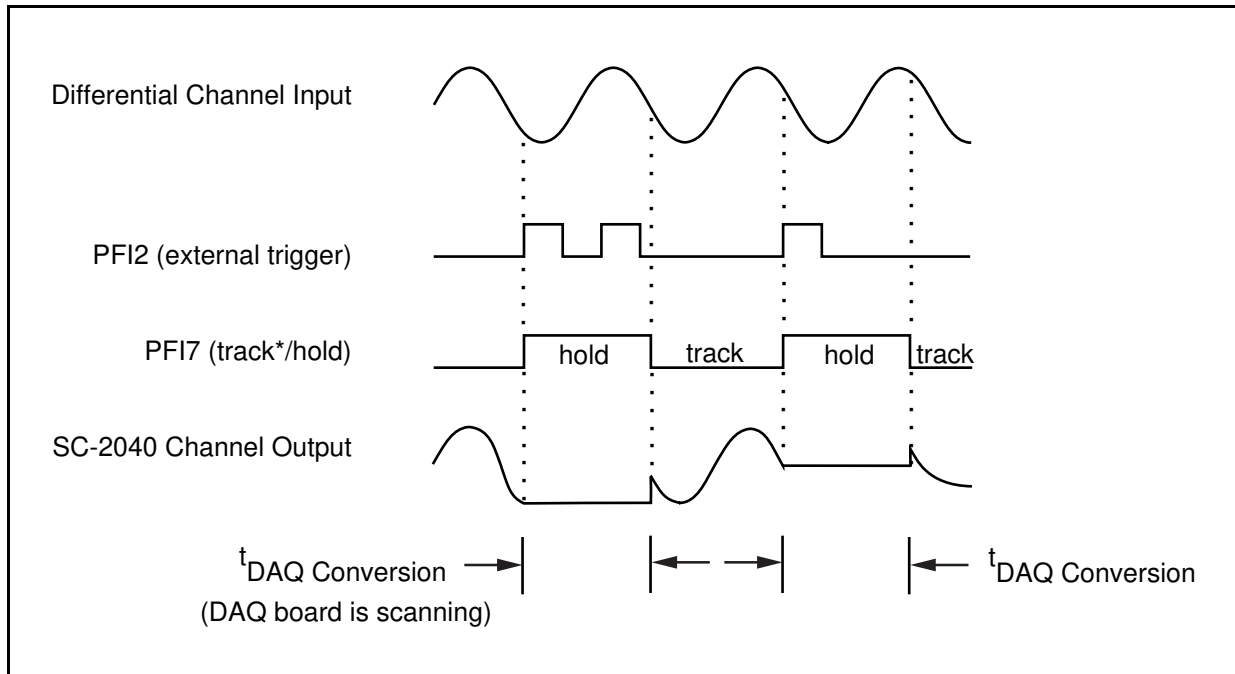


Figure 4-4. External Triggering

Output Connection

The output of every channel is connected to the 68-pin rear signal connector and the 50-pin supplemental I/O connector. The 68-pin connector carries signals to and from the DAQ board, and also provides +5 V power if selected by the power switch. The corresponding pins of the 50-pin connector are tied to those of the 68-pin connector so that you can monitor these signals on the 50-pin connector. The pin connections of these connectors are given in Chapter 3, *Signal Connections*.

Power Supply

The SC-2040 contains an onboard power switch to either power the SC-2040 from the MIO-16E board or to draw power from an external +5 V supply. From the +5 V power, an onboard DC-to-DC converter generates a ± 15 V source, which is used to power the analog circuitry. A red LED indicates that the board is receiving power.

Chapter 5

Calibration Procedures

This chapter discusses the calibration procedures for the SC-2040 board.

Note: *In many applications, the SC-2040 factory-hardware calibration is sufficient to meet accuracy requirements, and no further calibration, either hardware or software, is needed.*

Although hardware calibration is discussed in greater detail than software calibration, software calibration is the preferred choice for the following reasons:

- The calibration adjustments on the SC-2040 are inaccessible under most normal operating circumstances.
- With software calibration, the board is calibrated in the exact environment in which it will be operating. Software calibration compensates for system-introduced, in addition to board-introduced, errors. You can perform software calibration fairly frequently, which helps reduce drift effects.

Because board-introduced errors are minimal with the SC-2040, the use of software rather than hardware calibration does not significantly reduce dynamic range. The main drawback of software calibration is reduced throughput due to the increased processing time.

Software Calibration

Software calibration is very simple. Depending on your accuracy requirements, you may want to perform only offset adjustment; offset and gain adjustments; or offset, gain, and linearity adjustments.

Offset Adjustment

Offset adjustment requires you to apply an input signal of zero to the channel to be calibrated. *Zero input* can mean shorting the board inputs to zero, or it can mean applying zero excitation to the transducer being used. In the former case, you can remove only board and DAQ board offset; in the latter case, transducer offset is removed as well. In either case, measurements are taken with the zero input signal. Average these measurements to reduce uncertainty. This average represents the offset. Next, subtract the offset from all subsequent measurements. Notice that offset changes with gain; thus, during calibration, set the channel to the gain at which the subsequent measurements will be taken.

Gain Adjustment

Gain adjustment requires you to apply two different input signals. One of the two points is typically zero, because zero is easy to generate with a high degree of accuracy. The other should be near full scale, either a DC-voltage from a precision calibrator or a voltage generated by applying a known excitation to the transducer being used. Of course, you should generate both signals—zero and full scale—from the same source.

Take measurements on both signals and compute separate averages. Then combine the averages with the known input signals to generate linear correction factors for all subsequent measurements. Specifically, if the input X yields measurement x , and the input Y yields measurement y , then you should process measurement z as shown in the following equation to yield the corrected measurement Z :

$$Z = X + \frac{(Y - X)(z - x)}{(y - x)}.$$

Linearity Adjustment

The SC-2040 seldom needs linearity adjustment because its linearity is quite good, especially at low gains. Linearity error is often caused by the nonlinearity of the DAQ board you use. If necessary, the method described previously for correcting gain and offset error may be extended to include linearity by taking more points along the transfer function and processing the subsequently acquired data according to a polynomial fit of the calibration points.

Alternatively, and preferably for DAQ boards with no more than 12 bits of resolution, you can determine the nonlinearity of the system on a code-by-code basis, and you can subtract the error of each code from any measurement that returns that value. This method has the advantage of correcting differential as well as integral linearity errors. However, this method may be time-consuming. If time permits, you may determine the nonlinearity of your system on a code-by-code basis with even higher resolution DAQ boards. Describing methods of measuring system nonlinearity is beyond the scope of this manual. If linearity correction becomes necessary, refer to your DAQ board user manual.

Hardware Calibration

There are two potentiometers (pots) to adjust for each channel. These are set at the factory and should not need to be readjusted for most applications. The pots adjust input offset voltage and output offset voltage for each of the eight channels. Gain error and linearity are not adjustable. For detailed specifications of offset, gain, and linearity error, see Appendix A, *Specifications*.

Input offset is any error voltage that appears to be added to the input signal; that is, its effect is multiplied by the gain of the instrumentation amplifier. Output offset is any error voltage that appears to be added to the output signal; that is, its effect is independent of the gain of the instrumentation amplifier. At a fixed gain, these errors are indistinguishable; thus, it is necessary to switch between gains to properly calibrate the SC-2040.

Your accuracy needs determine how carefully the offsets need to be calibrated. A typical requirement might be for total offset referred to output to be less than half of an LSB of the DAQ board being used. For example, a 12-bit, 20 V system has a resolution of $20 \text{ V}/2^{12} = 4.88 \text{ mV}$. Calibration to under 2 mV would thus be sufficient for most applications. The SC-2040 is factory calibrated to have total offset referred to output of less than 2 mV at low gains.

Table 5-1 shows which pots to adjust for each type of offset for each channel and which DIP switch selects the gain for each channel. Refer to the parts locator diagram in Chapter 2, *Configuration and Installation*, to determine the location of each component.

Table 5-1. Calibration Component Identification

| Channel | Output Offset Adjust | Input Offset Adjust | Gain DIP Switch |
|---------|----------------------|---------------------|-----------------|
| 0 | R1 | R4 | U2 |
| 1 | R7 | R11 | U6 |
| 2 | R13 | R16 | U9 |
| 3 | R18 | R22 | U14 |
| 4 | R25 | R29 | U17 |
| 5 | R32 | R35 | U21 |
| 6 | R37 | R41 | U24 |
| 7 | R45 | R48 | U28 |

A complicating factor in the calibration of the board is that the output offset is not the same in track mode as in hold mode. This difference is because of a phenomenon known as *hold step*, in which a small amount of charge is transferred to the track-and-hold amplifier hold capacitor during the transition from track mode to hold mode. This charge transfer slightly changes the voltage at the output of the track-and-hold amplifier.

The magnitude of the *hold step* on the SC-2040 is approximately 5 mV, enough to make it necessary to calibrate output offset in hold mode rather than track mode. You may calibrate input offset without switching the board to hold mode.

To calibrate the SC-2040 board, the following steps are required:

1. If you are using a rack-mount kit, remove the cover to expose the DIO switches and jumpers. Connect the board so that the pots and DIP switches are readily accessible.
2. Short each input of the board to ground.

At low gains, more alternatives exist to serve as a short circuit, but at a gain of 500, 1 mV referred to the output is only 2 μV referred to the input. Thermoelectric effects make it difficult to keep a short circuit from generating such voltages. The best solution is to use short lengths of heavy copper wire, and to keep the short away from heat sources.

3. Program the DAQ board to take data in the differential input mode.

The SC-2040 should switch between track mode and hold mode, with the DAQ board sampling occurring while the board is in hold mode.

4. Set the DAQ board to a high gain and measure its offset by shorting its input.

You must subtract this measured offset from all subsequent board measurements to ensure accuracy.

For the offset of the DAQ board not to affect the calibration, you must subtract the offset from all board offset measurements. Thus, you must first measure the offset to an accuracy better than that to which the board is to be calibrated. Furthermore, setting the DAQ board to a high gain (100, for example) makes it possible to resolve offset changes that would be indiscernible at lower gains. Because the DAQ board offset will not be independent of gain, you should set the gain first, and then measure the offset. To measure the offset, disconnect the board from the DAQ board, short circuit the board inputs to ground, and take some data. The measured value is the offset. For a reliable value, use software to average a few hundred readings. After you have measured and recorded the offset, remove the short circuits and reconnect the board.

5. Measure the output of the first channel with its gain set to one and adjust its output offset pot until the output is close to zero.

At this gain, most of the board offset is due to output offset. The input offset adjustment has minimal effect. Set the DAQ board to read the channel. Acquire the data, averaging as in step 4. Adjust the output offset pot until the difference between the measured offset and the DAQ board offset is close to zero. There is no need to adjust it perfectly because the input offset adjustment in the next step might make a slight change in the measured gain-of-one offset.

6. Measure the output of the same channel with its gain set to 500 and adjust its input offset pot until the output is close to zero.

At this gain, the input offset adjustment has the dominant effect. Acquire the data and average as before. Adjust the input offset pot until the difference between the measured offset and the DAQ board offset is close to zero. Again, it is not necessary to adjust the input offset perfectly because there will be a slight interdependence between the two offsets.

7. Repeat step 5, adjusting the offset as carefully as desired. Then repeat step 6, adjusting the offset as carefully as desired. Switch back to a gain of one to ensure that the low-gain offset is still calibrated. If necessary, repeat steps 5 and 6 until the offset is calibrated at both gains.
8. Repeat steps 5 through 7 for the additional channels you want to calibrate. There is no calibration interdependence among the channels.
9. Replace the rack-mount chassis cover, if used.

Appendix A

Specifications

This appendix lists the specifications for the SC-2040. These are typical at 25° C unless otherwise stated. The operating temperature range is 0° to 50° C.

Analog Input

Input Characteristics

Number of channels 8 differential

Input signal ranges

| Board Gain (Hardware Selectable) | Board Range Max Output Range ± 10 V |
|-------------------------------------|--|
| 1 | ± 10 V |
| 10 | ± 1 V |
| 100 | ± 100 mV |
| 200 | ± 50 mV |
| 300 | ± 33.3 mV |
| 500 | ± 20 mV |
| 600 | ± 16.67 mV |
| 700 | ± 14.29 mV |
| 800 | ± 12.5 mV |

Input coupling

DC

Max working voltage
(signal + common mode)

Average of 2 inputs should remain within ± 7 V of ground

Overvoltage protection

± 30 V powered on, ± 15 V powered off

Inputs protected

ACH<0..7>

Transfer Characteristics

Offset error

Pregain error after calibration

± 100 μ V max

Postgain error after calibration

± 2 mV max

Gain error and nonlinearity

| Gain (DIP-switch-selectable) | Max Gain Error | Max Gain Tempco | Max Nonlinearity |
|---------------------------------|--------------------|-----------------------------|---------------------|
| 1 | $\pm 0.05\%$ | ± 25 ppm/ $^{\circ}$ C | $\pm 0.01\%$ |
| 10 | $\pm 0.1\%$ | ± 25 ppm/ $^{\circ}$ C | $\pm 0.01\%$ |
| 100 | $\pm 0.2\%$ | ± 45 ppm/ $^{\circ}$ C | $\pm 0.02\%$ |
| 200 | $\pm 0.4\%$ | ± 60 ppm/ $^{\circ}$ C | $\pm 0.02\%$ |
| 300 | -0.3%, $\pm 0.6\%$ | ± 80 ppm/ $^{\circ}$ C | $\pm 0.03\%$ |
| 500 | $\pm 1.0\%$ | ± 100 ppm/ $^{\circ}$ C | $\pm 0.04\%$ |
| 600 | -0.2%, $\pm 1.5\%$ | ± 120 ppm/ $^{\circ}$ C | $\pm 0.05\%$ |
| 700 | -0.1%, $\pm 2.0\%$ | ± 150 ppm/ $^{\circ}$ C | $\pm 0.06\%$ |
| 800 | -0.3%, $\pm 3.0\%$ | ± 200 ppm/ $^{\circ}$ C | $\pm 0.07\%$ |

Amplifier Characteristics

Input impedance
 Normal powered on 100 GΩ in parallel with 20 pF
 Input bias current ±100 pA, ±10 mA max
 Input offset current ±10 pA

CMRR

| Gain | dB (min and typ) |
|------------|------------------------|
| Gain = 1 | 70 dB min, 90 dB typ |
| Gain = 10 | 87 dB min, 104 dB typ |
| Gain ≥ 100 | 100 dB min, 110 dB typ |

Output range ±10 V

Dynamic Characteristics

Bandwidth

| Gain | -3 dB Bandwidth |
|------|-----------------|
| 1 | 2 MHz |
| 10 | 800 kHz |
| 100 | 500 kHz |
| 200 | 300 kHz |
| 300 | 180 kHz |
| 500 | 120 kHz |
| 600 | 100 kHz |
| 700 | 80 kHz |
| 800 | 70 kHz |

System noise

| Gain | Filter |
|------|-----------|
| 1 | 175 μVrms |
| 10 | 50 μVrms |
| 100 | 45 μVrms |
| 200 | 40 μVrms |
| 300 | 35 μVrms |
| 500 | 33 μVrms |
| 600 | 30 μVrms |
| 700 | 29 μVrms |
| 800 | 27 μVrms |

Noise spectral density
 Input noise (gain = 1) 12 nV/√Hz
 Output noise 85 nV/√Hz
 Slew rate 8 V/μs

S/H Characteristics

| Measurement | 0.012% | 0.003% | 0.0015% | 0.00076% |
|-----------------------------|---------------|------------|------------|-----------|
| Track mode acquisition time | 7 μ s | 10 μ s | 50 μ s | 1 ms |
| Hold mode settling time | 1 μ s | 1 μ s | 1 μ s | 2 μ s |
| Hold step | -5 mV | — | — | — |
| Droop rate | ± 10 mV/s | — | — | — |
| Aperture time | 250 ns | — | — | — |
| Interchannel skew | ± 50 ns | — | — | — |

Stability

Recommended warm-up time
Offset temperature coefficient

15 min
 $\pm(10 + 150/\text{gain}) \mu\text{V}/^\circ\text{C}$

Gain temperature coefficient

| Gain (DIP-switch-selectable) | Max Gain Tempco |
|---------------------------------|---------------------------------|
| 1 | ± 25 ppm/ $^\circ\text{C}$ |
| 10 | ± 25 ppm/ $^\circ\text{C}$ |
| 100 | ± 45 ppm/ $^\circ\text{C}$ |
| 200 | ± 60 ppm/ $^\circ\text{C}$ |
| 300 | ± 80 ppm/ $^\circ\text{C}$ |
| 500 | ± 100 ppm/ $^\circ\text{C}$ |
| 600 | ± 120 ppm/ $^\circ\text{C}$ |
| 700 | ± 150 ppm/ $^\circ\text{C}$ |
| 800 | ± 200 ppm/ $^\circ\text{C}$ |

Power Requirement

+5 VDC (± 10 %)
Total power dissipation

800 mA
4 W

Physical

Dimensions
I/O connectors
 Input
 Output

1.8 by 7.9 by 4.9 in. (4.6 by 20.1 by 12.4 cm)
20-screw terminals
50-pin male ribbon-cable rear connector
68-pin male ribbon-cable rear connector

Environment

Operating temperature
Storage temperature
Relative humidity

0 $^\circ$ to 50 $^\circ$ C
-55 $^\circ$ to 150 $^\circ$ C
5% to 90% noncondensing

Appendix B

Customer Communication

For your convenience, this appendix contains forms to help you gather the information necessary to help us solve technical problems you might have as well as a form you can use to comment on the product documentation. Filling out a copy of the *Technical Support Form* before contacting National Instruments helps us help you better and faster.

National Instruments provides comprehensive technical assistance around the world. In the U.S. and Canada, applications engineers are available Monday through Friday from 8:00 a.m. to 6:00 p.m. (central time). In other countries, contact the nearest branch office. You may fax questions to us at any time.

Corporate Headquarters

(512) 795-8248

Technical support fax: (800) 328-2203
(512) 794-5678

| Branch Offices | Phone Number | Fax Number |
|-----------------------|---------------------|-------------------|
| Australia | (03) 879 9422 | (03) 879 9179 |
| Austria | (0662) 435986 | (0662) 437010-19 |
| Belgium | 02/757.00.20 | 02/757.03.11 |
| Denmark | 45 76 26 00 | 45 76 71 11 |
| Finland | (90) 527 2321 | (90) 502 2930 |
| France | (1) 48 14 24 00 | (1) 48 14 24 14 |
| Germany | 089/741 31 30 | 089/714 60 35 |
| Italy | 02/48301892 | 02/48301915 |
| Japan | (03) 3788-1921 | (03) 3788-1923 |
| Netherlands | 03480-33466 | 03480-30673 |
| Norway | 32-848400 | 32-848600 |
| Spain | (91) 640 0085 | (91) 640 0533 |
| Sweden | 08-730 49 70 | 08-730 43 70 |
| Switzerland | 056/20 51 51 | 056/20 51 55 |
| U.K. | 0635 523545 | 0635 523154 |

Technical Support Form

Photocopy this form and update it each time you make changes to your software or hardware, and use the completed copy of this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

If you are using any National Instruments hardware or software products related to this problem, include the configuration forms from their user manuals. Include additional pages if necessary.

Name _____

Company _____

Address _____

Fax (____) _____ Phone (____) _____

Computer brand _____ Model _____ Processor _____

Operating system _____

Speed _____MHz RAM _____MB Display adapter _____

Mouse _____yes _____no Other adapters installed _____

Hard disk capacity _____MB Brand _____

Instruments used _____

National Instruments hardware product model _____ Revision _____

Configuration _____

National Instruments software product _____ Version _____

Configuration _____

The problem is _____

List any error messages _____

The following steps will reproduce the problem _____

SC-2040 Hardware and Software Configuration Form

Record the settings and revisions of your hardware and software on the line to the right of each item. Complete a new copy of this form each time you revise your software or hardware configuration, and use this form as a reference for your current configuration. Completing this form accurately before contacting National Instruments for technical support helps our applications engineers answer your questions more efficiently.

National Instruments Products

- DAQ Hardware Revision _____
- Interrupt Level of Hardware _____
- DMA Channels of Hardware _____
- Base I/O Address of Hardware _____
- NI-DAQ Version _____

Other Products

- Computer Make and Model _____
- Microprocessor _____
- Clock Frequency _____
- Type of Video Board Installed _____
- Operating System _____
- Operating System Version _____
- Operating System Mode _____
- Programming Language _____
- Programming Language Version _____
- Other Boards in System _____
- Base I/O Address of Other Boards _____
- DMA Channels of Other Boards _____
- Interrupt Level of Other Boards _____

Documentation Comment Form

National Instruments encourages you to comment on the documentation supplied with our products. This information helps us provide quality products to meet your needs.

Title: **SC-2040 User Manual**

Edition Date: **September 1994**

Part Number: **371191A-01**

Please comment on the completeness, clarity, and organization of the manual.

If you find errors in the manual, please record the page numbers and describe the errors.

Thank you for your help.

Name _____

Title _____

Company _____

Address _____

Phone (_____) _____

Mail to: Technical Publications
National Instruments Corporation
6504 Bridge Point Parkway, MS 53-02
Austin, TX 78730-5039

Fax to: Technical Publications
National Instruments Corporation
MS 53-02
(512) 794-5678

Glossary

| Prefix | Meaning | Value |
|--------|---------|-------------------|
| p- | pico- | 10 ⁻¹² |
| n- | nano- | 10 ⁻⁹ |
| μ- | micro- | 10 ⁻⁶ |
| m- | milli- | 10 ⁻³ |
| k- | kilo- | 10 ³ |
| M- | mega- | 10 ⁶ |

| | |
|------------------|--|
| ° | degrees |
| Ω | ohms |
| A | amperes |
| ACH# | DAQ board analog input channel number |
| A/D | analog-to-digital |
| Arms | amperes, root mean square |
| AWG | American Wire Gauge |
| C | Celsius |
| CH#+ | module positive input channel number |
| CH#- | module negative input channel number |
| CMOS | complementary metallic oxide semiconductor |
| cps | counts per second |
| D/A | digital-to-analog |
| DAQ | data acquisition |
| dB | decibels |
| DC | direct current |
| DIN | Deutsche Industrie Norme |
| DIP | dual inline package |
| FIFO | first-in-first-out |
| hex | hexadecimal |
| Hz | hertz |
| in. | inches |
| I _I | input current leakage |
| I _{in} | input current |
| I/O | input/output |
| I _{out} | output current |
| LED | light-emitting diode |
| LSB | least significant bit |
| m | meters |
| MB | megabytes |
| MSB | most significant bit |
| ppm | parts per million |

Glossary

| | |
|------------------|-----------------------------|
| RAM | random-access memory |
| rms | root mean square |
| s | seconds |
| SPI | serial peripheral interface |
| tempco | temperature coefficient |
| T/H | track-and-hold |
| UL | Underwriters Laboratory |
| V | volts |
| VI | virtual instrument |
| V _{IH} | volts input high |
| V _{IL} | volts input low |
| V _{in} | volts in |
| V _{OH} | volts output high |
| V _{OL} | volts output low |
| V _{out} | volts out |
| VAC | volts alternating current |
| VDC | volts direct current |
| V _{rms} | volts, root mean square |

Index

Numbers/Symbols

+5 V signal
input connector summary (table), 3-4
output connector summary (table), 3-4 to 3-5

A

AC-coupled inputs, 3-8 to 3-11
common-mode input range, 3-10 to 3-11
exceeding differential and common-mode ranges (warning), 3-10
floating AC-coupled signal connection (illustration), 3-8
ground-offset AC-coupled signal connection (illustration), 3-9
ground-referenced AC-coupled signal connection (illustration), 3-9
referencing analog ground to DAQ board (note), 3-8
AIGND-AIGND position (table), 2-4
AIGND-DGND position (table), 2-4
AIGND signal
input connector summary (table), 3-4
output connector summary (table), 3-4 to 3-5
analog circuitry, 4-2 to 4-6
amplification, 4-3
external triggering, 4-5 to 4-6
input protection, 4-3
output connection, 4-6
power supply, 4-6
track-and-hold (T/H) circuitry, 4-3 to 4-4
triggering from DAQ board, 4-4 to 4-5
analog input specifications
amplifier characteristics, A-2
dynamic characteristics, A-2
input characteristics, A-1
S/H characteristics, A-3
stability, A-3
transfer characteristics, A-1
analog signal inputs, 3-7 to 3-11
AC-coupled inputs, 3-8 to 3-11

common-mode input range, 3-10 to 3-11
exceeding differential and common-mode ranges (warning), 3-10
floating AC-coupled signal connection (illustration), 3-10
ground-offset AC-coupled signal connection (illustration), 3-9
ground-referenced AC-coupled signal connection (illustration), 3-9
referencing analog ground to DAQ board (note), 3-8
analog input ranges, 3-10 to 3-11
DC-coupled inputs, 3-7 to 3-8
floating signal connection (illustration), 3-8
ground-referenced signal connection (illustration), 3-7
leaving connector J5 disconnected (note), 3-7

B

block diagram of SC-2040, 4-2
board configuration. *See* configuration.

C

calibration procedures
hardware calibration, 5-2 to 5-4
calibration component identification (table), 5-3
steps for, 5-3 to 5-4
overview, 5-1
software calibration
gain adjustment, 5-2
linearity adjustment, 5-2
offset adjustment, 5-1
CH-(0..7) signal (table), 3-3
channel gain selection
gain switches for each channel (table), 2-6

- procedure for, 2-6 to 2-7
 - switch settings (table), 2-7
 - table, 2-5
- channel input mode (table), 2-5
- CH+(0..7) signal (table), 3-4
- common-mode input range, 3-10 to 3-11
- configuration
 - channel gain selection
 - gain switches for each channel (table), 2-6
 - procedure for, 2-6 to 2-7
 - switch settings (table), 2-7
 - table, 2-5
 - channel input mode (table), 2-5
 - DAQ board ground isolation selection
 - procedure for, 2-6
 - table, 2-4
 - input mode selection, 2-7
 - parts locator diagram, 2-2
 - power supply selection
 - procedure for, 2-6
 - table, 2-3
 - shield selection
 - procedure for, 2-4
 - table, 2-4
- connectors J11 and J12
 - overview, 3-1
 - pin assignments (illustration), 3-2 (table), 3-3
 - signal routing (illustration), 3-6
 - signal summary (table), 3-4
- customer communication, *xi*, B-1

D

- DAQ board ground isolation selection
 - procedure for, 2-6
 - table, 2-4
- DC-coupled inputs, 3-7 to 3-8
 - floating signal connection (illustration), 3-8
 - ground-referenced signal connection (illustration), 3-7
 - leaving connector J5 disconnected (note), 3-7
- DGND signal
 - input connector summary (table), 3-4

- output connector summary (table), 3-4 to 3-5
- digital signal inputs, 3-9
- documentation
 - conventions used in manual, *x*
 - National Instruments documentation set, *x*
 - organization of manual, *ix*
 - related documentation, *xi*

E

- environment specifications, A-3
- equipment, optional, 1-4
- EXT switch position (table), 2-3

F

- floating AC-coupled signal connection (illustration), 3-10
- floating signal connection (illustration), 3-8

G

- gain selection. *See* channel gain selection.
- ground-offset AC-coupled signal connection (illustration), 3-9
- ground-referenced AC-coupled signal connection (illustration), 3-9
- ground-referenced signal connection (illustration), 3-7

H

- hardware calibration.
 - See* calibration procedures.
- hold-mode settling time, 4-3

I

- input connectors signal summary (table), 3-4
- input mode selection, 2-7
- installation
 - power-on sequence, 2-8
 - steps for, 2-8

unpacking the SC-2040, 1-4
instrumentation amplifiers, 4-3
INT switch position (table), 2-3

J

J11 and J12 connectors. *See* connectors J11 and J12.

jumpers and switches. *See* configuration.

L

LabVIEW and LabWindows application software, 1-2

M

manual. *See* documentation.

MIO-16E DAQ board, triggering, 4-4 to 4-5

monitoring signal inputs, 3-11

O

operation of SC-2040. *See* theory of operation.

output connection, 4-6

output connectors (J11 and J12) signal summary (table), 3-4 to 3-5

P

parts locator diagram, 2-2

physical specifications, A-3

pin assignments for SC-2040 I/O connectors J11 and J12 (table), 3-3

power-on sequence, 2-8

power supply

description, 4-6

selecting

procedure for, 2-6

table, 2-3

specifications, A-3

R

register-level programming, 1-4

S

SC-2040

block diagram, 4-2

features, 1-1

I/O connectors (J11 and J12), (illustration), 3-2

optional equipment, 1-4

required components, 1-1

software programming choices

LabVIEW and LabWindows

application software, 1-2

NI-DAQ driver software, 1-2 to 1-3

register-level programming, 1-4

unpacking, 1-4

shield selection

procedure for, 2-4

table, 2-4

SHLD OFF jumper position (table), 2-4

SHLD ON jumper position (table), 2-4

signal connections

analog signal inputs, 3-7 to 3-1

AC-coupled inputs, 3-10 to 3-11

analog input ranges, 3-10 to 3-11

DC-coupled inputs, 3-7 to 3-8

connections exceeding maximum ratings (warning), 3-1

digital signal inputs, 3-11

input connectors signal summary

(table), 3-4

monitoring signal inputs, 3-11

other connection considerations, 3-11

output connectors (J11 and J12) signal summary (table), 3-4 to 3-5

SC-2040 I/O connectors J11 and J12 (illustration), 3-2

signal routing (illustration), 3-6

signal outputs, monitoring, 3-11

software calibration.

See calibration procedures.

software programming choices

LabVIEW and LabWindows application software, 1-2

NI-DAQ driver software, 1-2 to 1-3

- register-level programming, 1-4
- specifications
 - analog input
 - amplifier characteristics, A-2
 - dynamic characteristics, A-2
 - input characteristics, A-1
 - S/H characteristics, A-3
 - stability, A-3
 - transfer characteristics, A-1
 - environment, A-3
 - physical, A-3
 - power requirements, A-3

T

- technical support, B-1
- theory of operation
 - analog circuitry, 4-2 to 4-6
 - amplification, 4-3
 - external triggering, 4-5 to 4-6
 - input protection, 4-3
 - output connection, 4-6
 - power supply, 4-6
 - track-and-hold (T/H) circuitry, 4-3 to 4-4
 - triggering from DAQ board, 4-4 to 4-5
 - block diagram, 4-2
 - functional overview, 4-1
- track-and-hold (T/H) circuitry, 4-3 to 4-4
- TRIG signal
 - description (table), 3-4
 - susceptibility to noise, 3-11
- TRIG (PF12) signal (table), 3-4
- triggering
 - from DAQ board, 4-4 to 4-5
 - external
 - digital signal inputs, 3-11
 - illustration, 4-6
 - theory of operation, 4-5 to 4-6

U

- unity gain position (table), 2-5
- unpacking the SC-2040, 1-4