

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

TB-2706

INSTALLATION GUIDE

NI TB-2706

PXI/PXIe Terminal Block for M Series and NI 6143 Devices

This installation guide describes how to install and connect signals to the NI TB-2706 terminal block for use with PXI/PXIe M Series, NI PXI-6143, and other PXI/PXIe devices with a 68-pin VHDCI connector.

Contents

Introduction.....	1
What You Need to Get Started	1
Safety Information	2
Connecting the Signals	3
Installing the Terminal Block	5
Specifications.....	6
Where to Go for Support	7

Introduction

The TB-2706 is a terminal block assembly consisting of a printed circuit board, 70 screw terminals, and a metal enclosure with strain relief hardware. The terminal block assembly connects directly to the front panel of National Instruments PXI-622x, PXI-625x, PXIe-625x, PXI-628x, and PXI-6143 devices, eliminating the need for an external cable.

The TB-2706 allows you to easily connect analog input, analog output, counter/timer, and digital I/O signals to your National Instruments device. The 70 screw terminals allow access to every pin on the connector, plus two shield screw terminals for use with a shielded cable. For M Series devices with two connectors, this terminal block allows access to every pin on Connector 0, plus two shield screw terminals for use with a shielded cable, but makes Connector 1 inaccessible.



Caution The TB-2706 is not designed for input voltages greater than $42 V_{pk}/60$ VDC, even if you install a voltage divider that reduces the voltage to within the input range of the DAQ device. Input voltages greater than $42 V_{pk}/60$ VDC can damage the TB-2706, any device connected to it, and the host computer. Overvoltage also can cause an electric shock hazard for the operator. National Instruments is *not* liable for damage or injury resulting from such misuse.

What You Need to Get Started

You need the following to set up and use your terminal block:

- ☐ NI TB-2706 Terminal Block Assembly
- ☐ *NI TB-2706 Installation Guide*
- ☐ NI PXI/PXIe M Series device, NI PXI-6143, or other PXI/PXIe device with a 68-pin VHDCI connector
- ☐ *M Series User Manual*, *S Series User Manual*, or other PXI/PXIe DAQ device documentation

- ☐ 0.10 in. slotted screwdriver
- ☐ Pinout label for M Series (adhered to cover of TB-2706) or pinout list for NI PXI-6143
- ☐ Number 1 Phillips screwdriver
- ☐ 26–16 AWG wire
- ☐ Wire cutters
- ☐ Wire insulation stripper

Safety Information



Cautions Do *not* operate the device in an explosive atmosphere or where there may be flammable gases or fumes.

Do *not* operate damaged equipment. The safety protection features built into this device can become impaired if the device becomes damaged in any way. If the device is damaged, turn the device off and do *not* use it until service-trained personnel can check its safety. If necessary, return the device to National Instruments for service and repair to ensure that its safety is not compromised.

Do *not* operate this equipment in a manner that contradicts the information specified in this document. Misuse of this equipment could result in a shock hazard.

Do *not* substitute parts or modify equipment. Because of the danger of introducing additional hazards, do *not* install unauthorized parts or modify the device. Return the device to National Instruments for service and repair to ensure that its safety features are not compromised.

You *must* insulate all of your signal connections to the highest voltage with which the TB-2706 can come in contact.

Connections, including power signals to ground and vice versa, that exceed any of the maximum signal ratings on the terminal block can create a shock or fire hazard, or can damage any or all of the boards connected to the host computer, and the terminal block. National Instruments is *not* liable for any damages or injuries resulting from incorrect signal connections.

Clean the module and accessories by brushing off light dust with a soft non-metallic brush. Remove other contaminants with a stiff non-metallic brush. The unit *must* be completely dry and free from contaminants before returning it to service.

Connecting the Signals

Refer to Figure 1 as you complete the following steps to connect signals to your terminal block.

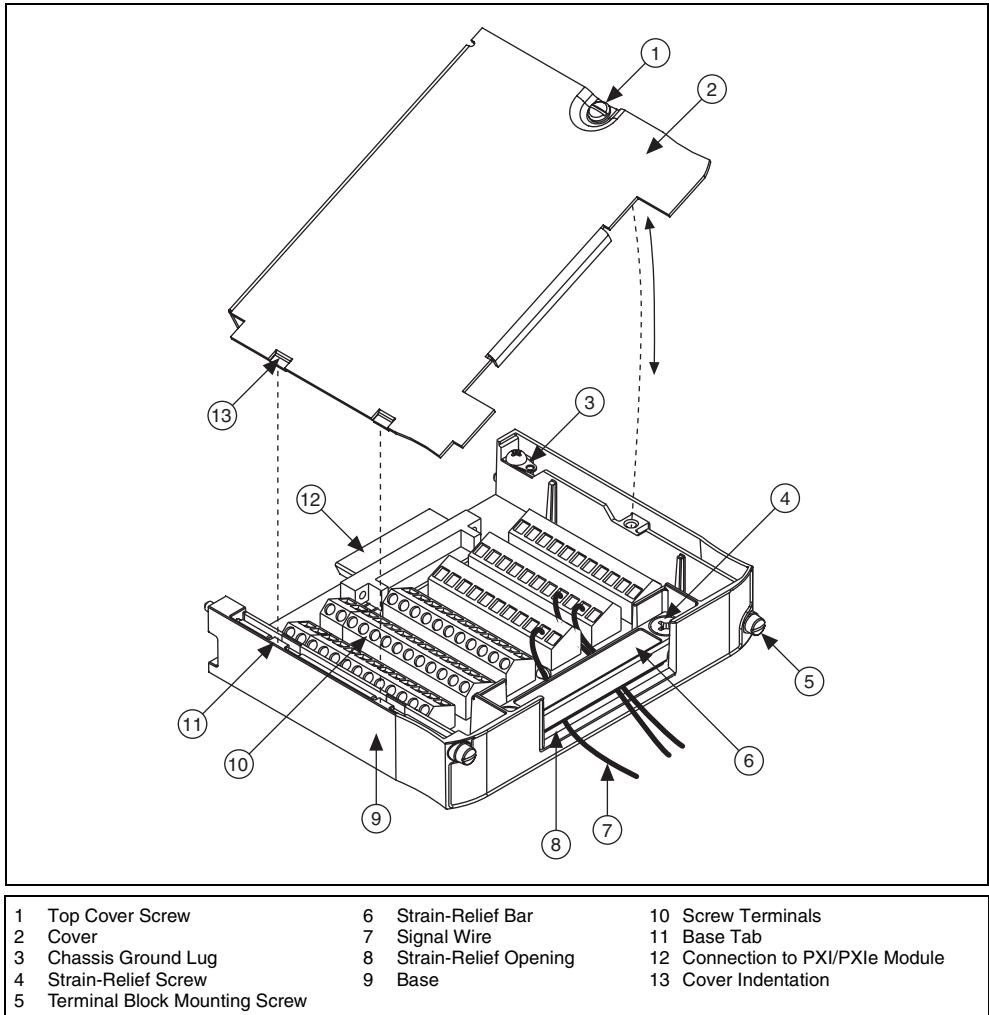


Figure 1. TB-2706 Parts Locator Diagram

1. Remove the terminal block cover by unscrewing the top cover screw using the 0.10 in. slotted screwdriver.



Note Your kit contains a pinout label for M Series devices only, shown in Figure 2. This label, adhered to the inside of the cover, is a pin number-to-signal name reference. For PXI-6143 pin connections, refer to Figure 3 or the *S Series User Manual*.



NI TB-2706 Pinout for M Series

PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL
68	AI 0	-	SHIELD	62	AI SENSE	15	D GND	4	D GND
34	AI 8	-	SHIELD	59	AI GND	14	+5 V	3	PFI 9/P2.1
33	AI 1	66	AI 9	64	AI GND	13	D GND	2	PFI 12/P2.4
65	AI 2	31	AI 10	67	AI GND	12	D GND	1	PFI 14/P2.6
30	AI 3	63	AI 11	32	AI GND	11	PFI 0/P1.0	35	D GND
28	AI 4	61	AI 12	29	AI GND	10	PFI 1/P1.1	36	D GND
60	AI 5	26	AI 13	27	AI GND	9	D GND	37	PFI 8/P2.0
25	AI 6	58	AI 14	24	AI GND	8	+5 V	38	PFI 7/P1.7
57	AI 7	23	AI 15	18	D GND	7	D GND	39	PFI 15/P2.7
22	AO 0	55	AO GND	17	P0.1	6	PFI 5/P1.5	40	PFI 13/P2.5
21	AO 1	54	AO GND	16	P0.6	5	PFI 6/P1.6	41	PFI 4/P1.4
20	APFI 0	56	AI GND					52	P0.0
53	D GND	19	P0.4						

If you are using a shielded cable, connect the cable shield to the terminals labeled "shield."

Figure 2. Pinout Label for M Series

NI TB-2706 Pinout for PXI-6143

PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL	PIN#	SIGNAL
68	AI 0 +	-	SHIELD	62	NC	15	D GND	4	D GND
34	AI 0 -	-	SHIELD	59	AI 5 GND	14	+5 V	3	PFI 9/CTR 0 GATE
33	AI 1 +	66	AI 1 -	64	AI 2 GND	13	D GND	2	CTR 0 OUT
65	AI 2 +	31	AI 2 -	67	AI 0 GND	12	D GND	1	FREQ OUT
30	AI 3 +	63	AI 3 -	32	AI 1 GND	11	PFI 0/AI START TRIG	35	D GND
28	AI 4 +	61	AI 4 -	29	AI 3 GND	10	PFI 1/AI REF TRIG	36	D GND
60	AI 5 +	26	AI 5 -	27	AI 4 GND	9	D GND	37	PFI 8/CTR 0 SOURCE
25	AI 6 +	58	AI 6 -	24	AI 6 GND	8	+5 V	38	PFI 7/AI SAMP CLK
57	AI 7 +	23	AI 7 -	18	D GND	7	D GND	39	D GND
22	NC	55	NC	17	P0.1	6	PFI 5	40	CTR 1 OUT
21	NC	54	NC	16	P0.6	5	PFI 6	41	PFI 4/CTR 1 GATE
20	NC	56	AI 7 GND						
53	D GND	19	P0.4						

If you are using a shielded cable, connect the cable shield to the terminals labeled "shield."

Figure 3. Pinout for PXI-6143

- Loosen or remove the strain-relief bar by loosening the two strain-relief screws with the Phillips-head screwdriver.
- Use wire cutters and wire insulation strippers to strip no more than 7 mm of insulation from the wire ends.
- Loosen the screws in the screw terminals with the 0.10 in. slotted screwdriver.
- Insert the stripped wires into the screw terminals. Tighten the screws with the 0.10 in. slotted screwdriver. No bare wire should extend past the screw terminal. Exposed wire increases the risk of short circuits and failures.

6. Tighten or replace the strain-relief screws.
7. Replace the terminal block cover by sliding the indentations on the cover under the tabs on the base. Tighten the top cover screw.

Installing the Terminal Block

Refer to Figure 4 as you complete the following steps to connect the terminal block to the PXI/PXIe module I/O connector.

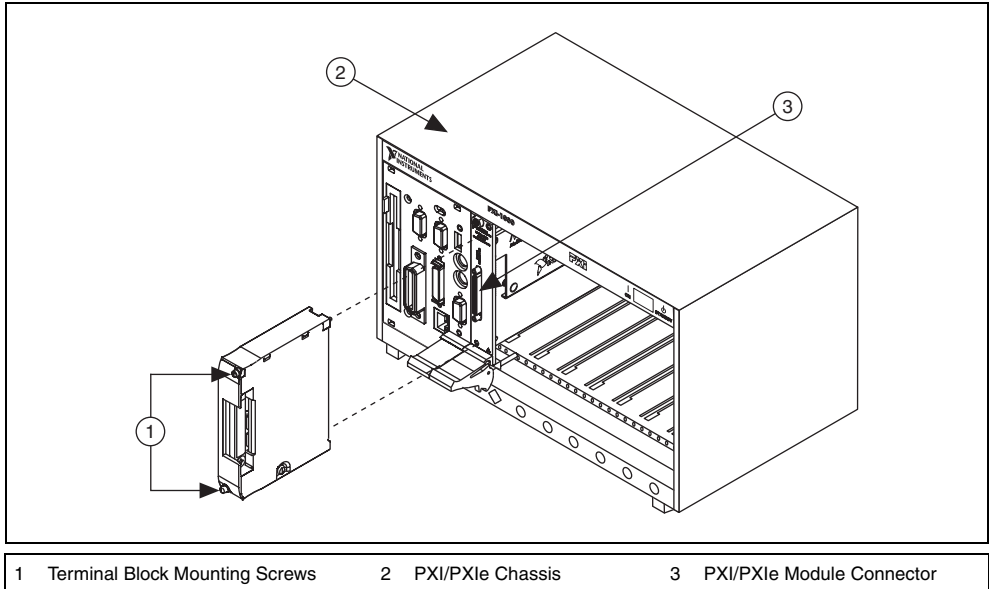


Figure 4. Connecting the TB-2706 to an M Series or PXI-6143 Device



Caution The connectors of both the PXI/PXIe module and the terminal block are polarized. You can attach them in only one way. Do *not* force the terminal block when inserting it into or removing it from the PXI/PXIe module I/O connector. Make sure that the chassis is powered off before inserting the PXI/PXIe module.

1. Install the PXI/PXIe module into the chassis and tighten the two module screws. You must install the TB-2706 terminal block on the PXI/PXIe module *after* the module is installed in the chassis.
2. Guide the terminal block onto the connector.
3. Tighten the two terminal block mounting screws.



Caution The TB-2706 is not designed for input voltages greater than $42 V_{pk}/60 \text{ VDC}$, even if you install a voltage divider that reduces the voltage to within the input range of the DAQ device. Input voltages greater than $42 V_{pk}/60 \text{ VDC}$ can damage the TB-2706, any device connected to it, and the host computer. Overvoltage also can cause an electric shock hazard for the operator. National Instruments is *not* liable for damage or injury resulting from such misuse.

Specifications

These specifications are typical at 25 °C unless otherwise specified.

Input/Output



Caution The TB-2706 is not designed for input voltages greater than 42 V_{pk}/60 VDC.

Refer to the documentation for your M Series or PXI-6143 device to determine the input/output specifications for your application.

Physical

Dimensions	10.7 × 8.6 × 2.0 cm (4.2 × 3.4 × 0.8 in.)
Dimension from face of PXI/PXIe card.....	8.6 cm (3.4 in.)
Weight	289 g (10.2 oz)
I/O connector	One 68-position male VHDCI connector
Screw terminals	
Number	70
Type.....	Angled entry, 3.81 mm pitch
Wire gauge	26–16 AWG

Environment

Operating temperature	0 to 55 °C
Storage temperature	–20 to 70 °C
Relative humidity	10 to 90% noncondensing
Pollution Degree (indoor use only).....	2
Altitude	2,000 m

Safety

This product is designed to meet the requirements of the following standards of safety for electrical equipment for measurement, control, and laboratory use:

- IEC 61010-1, EN 61010-1
- UL 61010-1, CSA 61010-1



Note For UL and other safety certifications, refer to the product label or visit ni.com/certification, search by model number or product line, and click the appropriate link in the Certification column.

Electromagnetic Compatibility

This product is designed to meet the requirements of the following standards of EMC for electrical equipment for measurement, control, and laboratory use:

- EN 61326 EMC requirements; Minimum Immunity
- EN 55011 Emissions; Group 1, Class A
- CE, C-Tick, ICES, and FCC Part 15 Emissions; Class A



Note For EMC compliance, operate this device according to product documentation.

CE Compliance

This product meets the essential requirements of applicable European Directives, as amended for CE marking, as follows:

- 73/23/EEC; Low-Voltage Directive (safety)
- 89/336/EEC; Electromagnetic Compatibility Directive (EMC)



Note Refer to the Declaration of Conformity (DoC) for this product for any additional regulatory compliance information. To obtain the DoC for this product, visit ni.com/certification, search by model number or product line, and click the appropriate link in the Certification column.

Waste Electrical and Electronic Equipment (WEEE)



EU Customers At the end of their life cycle, all products *must* be sent to a WEEE recycling center. For more information about WEEE recycling centers and National Instruments WEEE initiatives, visit ni.com/environment/weee.htm.

Where to Go for Support

The National Instruments Web site is your complete resource for technical support. At ni.com/support you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world to help address your support needs. For telephone support in the United States, create your service request at ni.com/support and follow the calling instructions or dial 512 795 8248. For telephone support outside the United States, contact your local branch office:

Australia 1800 300 800, Austria 43 662 457990-0, Belgium 32 (0) 2 757 0020,
Brazil 55 11 3262 3599, Canada 800 433 3488, China 86 21 5050 9800,
Czech Republic 420 224 235 774, Denmark 45 45 76 26 00, Finland 385 (0) 9 725 72511,
France 33 (0) 1 48 14 24 24, Germany 49 89 7413130, India 91 80 41190000, Israel 972 3 6393737,
Italy 39 02 413091, Japan 81 3 5472 2970, Korea 82 02 3451 3400, Lebanon 961 (0) 1 33 28 28,
Malaysia 1800 887710, Mexico 01 800 010 0793, Netherlands 31 (0) 348 433 466,
New Zealand 0800 553 322, Norway 47 (0) 66 90 76 60, Poland 48 22 3390150,
Portugal 351 210 311 210, Russia 7 495 783 6851, Singapore 1800 226 5886,
Slovenia 386 3 425 42 00, South Africa 27 0 11 805 8197, Spain 34 91 640 0085,
Sweden 46 (0) 8 587 895 00, Switzerland 41 56 2005151, Taiwan 886 02 2377 2222,
Thailand 662 278 6777, Turkey 90 212 279 3031, United Kingdom 44 (0) 1635 523545

National Instruments, NI, ni.com, and LabVIEW are trademarks of National Instruments Corporation. Refer to the *Terms of Use* section on ni.com/legal for more information about National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your CD, or ni.com/patents.