

COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs.

 Sell For Cash  Get Credit  Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock **New**, **New Surplus**, **Refurbished**, and **Reconditioned** NI Hardware.



Bridging the gap between the manufacturer and your legacy test system.

 1-800-915-6216

 www.apexwaves.com

 sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote

 **CLICK HERE**

USB-6001

USER GUIDE

NI USB-6001/6002/6003 OEM

This document provides information about the dimensions, pinouts, connectors, LEDs, and mounting holes of the National Instruments USB-6001/6002/6003 OEM device.


For more information about the device, refer to the *NI USB-6001/6002/6003 User Guide* and *NI USB-6001 Specifications*, *NI USB-6002 Specifications*, and *NI USB-6003 Specifications* documents available at ni.com/manuals.



Caution There are no product safety, electromagnetic compatibility (EMC), or CE marking compliance claims made for the NI USB-6001/6002/6003 OEM devices.

The NI USB-6001/6002/6003 OEM device is intended to be used as a component of a larger system. National Instruments can help developers meet their compliance requirements. The end product supplier, however, is responsible for conforming to any and all compliance requirements.

Figure 1. USB-6001/6002/6003 OEM Device

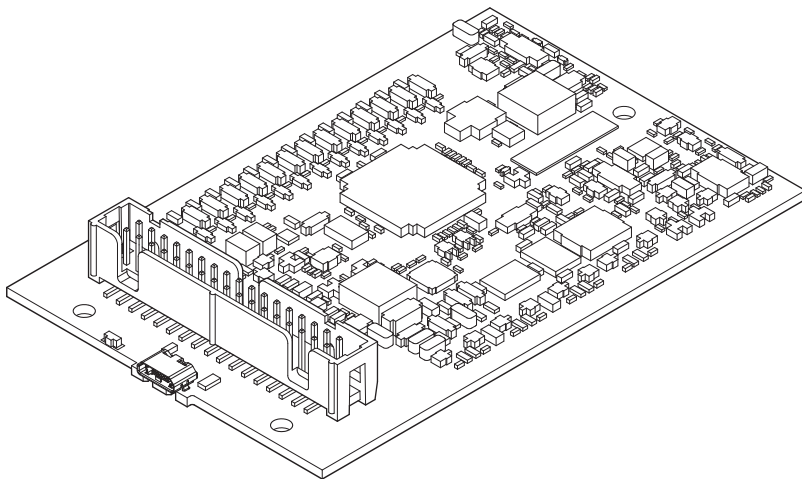


USB-6001/6002/6003 OEM Device Specifications

Most specifications of the USB-6001/6002/6003 OEM device are listed in the *NI USB-6001*, *NI USB-6002*, *NI USB-6003 Specifications* documents on ni.com/manuals. The following sections contain exceptions to the main specifications.

Physical Characteristics

Weight	31 g (1.10 oz)
Dimensions	98 mm × 64 mm × 12 mm (3.90 in. × 2.50 in. × 0.50 in.)

Figure 2. USB-6001/6002/6003 OEM Device Dimensions

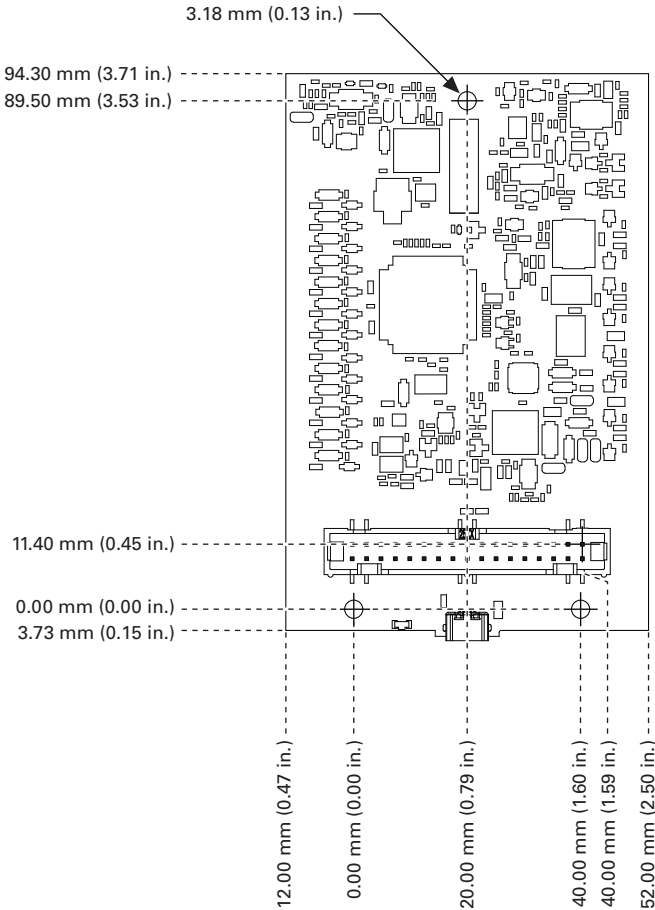

I/O Connector Pinouts

Figure 3 shows the USB-6001/6002/6003 OEM device I/O connector pinouts.

Figure 3. USB-6001/6002/6003 OEM Terminal Assignments

+5 V	34	33	P2.0/PFI 0
D GND	32	31	P1.3
P1.2	30	29	P1.1/PFI 1
P1.0	28	27	P0.7
P0.6	26	25	P0.5
P0.4	24	23	P0.3
P0.2	22	21	P0.1
P0.0	20	19	D GND
LED	18	17	D+
VBUS	16	15	D-
AI GND	14	13	AI GND
AI 4 (AI 0-)	12	11	AI 0 (AI 0+)
AI 5 (AI 1-)	10	9	AI 1 (AI 1+)
AI 6 (AI 2-)	8	7	AI 2 (AI 2+)
AI 7 (AI 3-)	6	5	AI 3 (AI 3+)
AI GND	4	3	AO GND
AO1	2	1	AO0

Signal Descriptions

Most of the signals available on the I/O connector are described in the *NI USB-6001/6002/6003 User Guide* document available for download at ni.com/manuals. Table 1 describes additional signals on the I/O connector of the OEM device.

Table 1. Additional Signal Descriptions


Signal Name	Reference	Direction	Description
VBUS	D GND	Input	USB Power
D+, D-	D GND	Input/Output	USB Data Lines
LED	D GND	Output	Status LED Driver

For more information about USB signals, refer to the *Universal Serial Bus Specification* accessible at www.usb.org.

Using the 34-Pin Connector with a Board Mount Socket

The USB-6001/6002/6003 OEM device can be mounted to a motherboard using the 34-pin connector, as shown in Figures 4 and 5.

Figure 4. Mounting Using a 34-Pin Connector

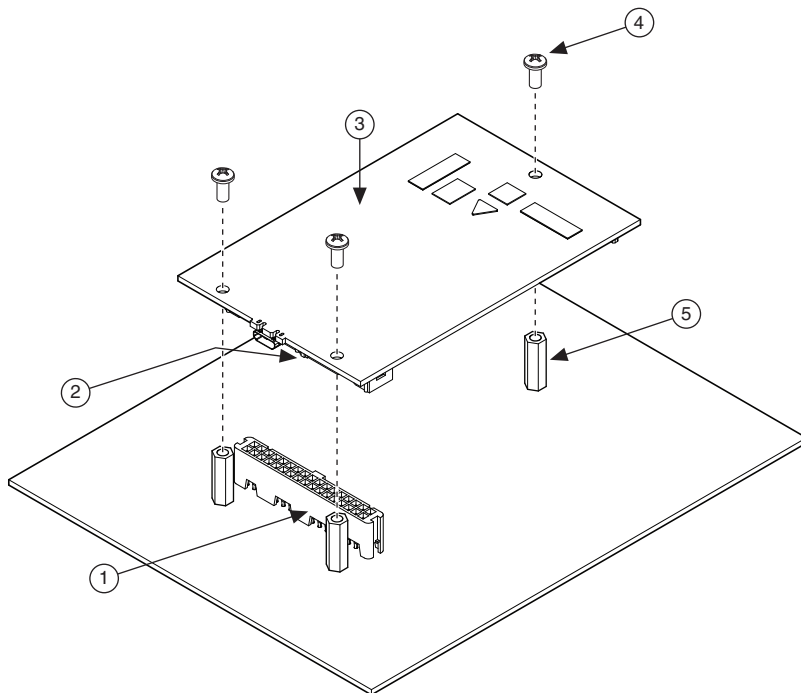


- 1 Board Mount Socket
- 2 34-Pin Connector
- 3 USB-6001/6002/6003 OEM Device

- 4 Mounting Screw
- 5 Mounting Standoff



Note Refer to the *Device Components* section for more information about mounting components.

Figure 5. USB Device Installed on Motherboard

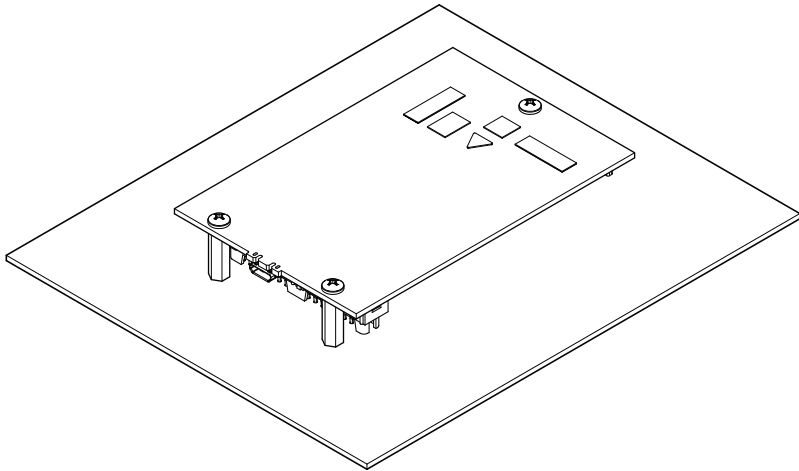

Connecting to USB

You can use the USB connector on the USB-6001/6002/6003 OEM device to connect to the USB host. In this case, leave the D+ and D- signals and VBUS (on the 34-pin connector) unconnected.


You can also use a USB connector on your motherboard to connect the USB-6001/6002/6003 OEM device to the USB host through the 34-pin connector. In this case, do not connect to the USB connector on the USB-6001/6002/6003 OEM device.

Using the Status LED Driver

The LED signal indicates the device status as listed in the *NI USB-6001/6002/6003 User Guide* document on ni.com/manuals. An open collector output drives the LED signal. For applications that use the LED signal, connect an external pull-up resistor from the LED signal to an external voltage.


To drive a status LED, refer to the circuit as shown in Figure 6.

Figure 6. To Drive a Status LED

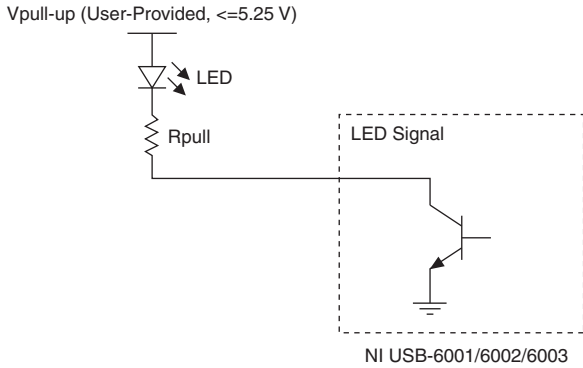

To use the LED signal to monitor the device state, refer to the circuit as shown in Figure 7.

Figure 7. To Monitor Device State Through the LED Signal

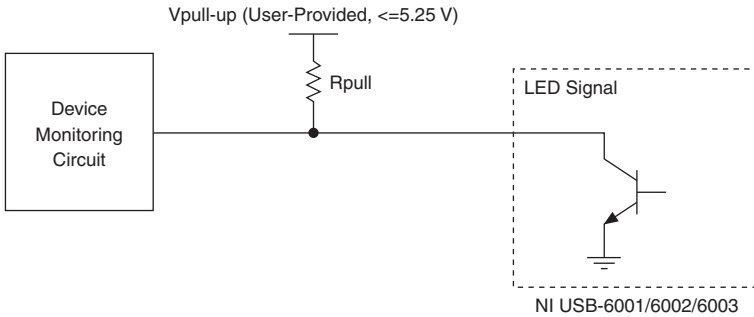

Electrical Characteristics

Table 2 lists the LED electrical characteristics.

Table 2. LED Electrical Characteristics

Parameter	Condition	Typical	Maximum
Output Low Voltage	$I_{OL} = 8 \text{ mA}$	—	0.4 V
	$I_{OL} = 18 \text{ mA}$	1.2 V	—
External Pull-up Voltage	—	—	5.25 V
Maximum Sinking Current	—	—	18 mA

Device Components

Table 3 lists the components used for interfacing and interacting with the USB-6001/6002/6003 OEM device.

Table 3. NI USB-6001/6002/6003 OEM Device Components

Component		Reference Designator(s) on PCB	Manufacturer	Manufacturer Part Number	Part Specifications
Micro USB connector		J001	Molex	105164-0001	—
Hi-Speed USB cable, A to Micro-B, 1 m		—	NI	782909-01	—
Hi-Speed USB cable, A to Micro-B, 2 m		—	NI	782909-02	—
34-pin connector		J002	3M	N2534-6V0C-RB-WF	—
34-pin mating connector		—	3M	8534-4500PL (or equivalent)	—
Mounting Standoff	Using 34-pin board mount socket	—	—	—	4.76 mm (3/16 in.) HEX female-to-female, 15 mm (0.59 in.) long
	Using ribbon cable	—	—	—	4.76 mm (3/16 in.) HEX female-to-female, 6.35 mm (1/4 in.) long
Screw		—	—	—	M3 × 0.5, 4-40 UNC

Worldwide Support and Services

The National Instruments website is your complete resource for technical support. At ni.com/support you have access to everything from troubleshooting and application development self-help resources to email and phone assistance from NI Application Engineers.

Visit ni.com/services for NI Factory Installation Services, repairs, extended warranty, and other services.

Visit ni.com/register to register your National Instruments product. Product registration facilitates technical support and ensures that you receive important information updates from NI.

National Instruments corporate headquarters is located at 11500 North Mopac Expressway, Austin, Texas, 78759-3504. National Instruments also has offices located around the world. For telephone support in the United States, create your service request at ni.com/support or dial 1 866 ASK MYNI (275 6964). For telephone support outside the United States, visit the Worldwide Offices section of ni.com/niglobal to access the branch office websites, which provide up-to-date contact information, support phone numbers, email addresses, and current events.

Refer to the *NI Trademarks and Logo Guidelines* at ni.com/trademarks for more information on National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: **Help»Patents** in your software, the `patents.txt` file on your media, or the *National Instruments Patents Notice* at ni.com/patents. You can find information about end-user license agreements (EULAs) and third-party legal notices in the readme file for your NI product. Refer to the *Export Compliance Information* at ni.com/legal/export-compliance for the National Instruments global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government Customers: The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015.

© 2014 National Instruments. All rights reserved.