COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series. We work out the best solution to suit your individual needs. We Sell For Cash We Get Credit We Receive a Trade-In Deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock New, New Surplus, Refurbished, and Reconditioned NI Hardware.

APEX WAVES

Bridging the gap between the manufacturer and your legacy test system.

1-800-915-6216
www.apexwaves.com
sales@apexwaves.com

All trademarks, brands, and brand names are the property of their respective owners.

Request a Quote CLICK HERE USB-6212



Manufacturer: National Instruments

Part Number and Revision	Description
194710A-04 or later	USB-6210
194710A-03 or later	USB-6211
196203A-03L or later	USB-6211 OEM
197493A-03L or later	USB-6212
198402A-03L or later	USB-6212 MASS TERMINATION
190630A-01L or later	USB-6212 BNC
197504A-03L or later	USB-6212 OEM
194710A-02 or later	USB-6215
197493A-01L or later	USB-6216
198402A-01L or later	USB-6216 MASS TERMINATION
190631A-01L or later	USB-6216 BNC
197504A-01L or later	USB-6216 OEM
194710A-01 or later	USB-6218
190632A-01L or later	USB-6218 BNC
196203A-01L or later	USB-6218 OEM

Volatile Memory

Target Data	Type	Size	Battery Backup	User ¹ Accessible	System Accessible	Sanitization Procedure
Glue logic	FPGA 1	Altera	No	No	Yes	Cycle Power
Glue logie	110/11	EP1C3	110	110	105	
Glue logic	FPGA 2	Xilinx	No	No	Yes	Cycle Power
		XC3S500E				
Program Code	SRAM	128 KB	No	No	Yes	Cycle Power

Non-Volatile Memory (incl. Media Storage)

Target Data	Туре	Size	Battery Backup	User Accessible	System Accessible	Sanitization Procedure
Device configuration	EEPROM	2 KB	No			
Device information				No	Yes	None
• Calibration metadata ²				Yes	Yes	Procedure 2
Calibration data				No	Yes	None

¹ Refer to *Terms and Definitions* section for clarification of *User* and *System Accessible*

 $^{^{2}}$ Calibration constants that are stored on the device include information for the device's full operating range. Any implications resulting from partial self-calibration can be eliminated by running the full self-calibration procedure.




Procedures


Procedure 1 – Board Assembly Part Number Identification:

To determine the Board Assembly Part Number and Revision, refer to the "P/N" label applied to the surface of your product as shown below. The Assembly Part Number should be formatted as "P/N: ######a-vvL" where "a" is the letter revision of the Board Assembly (eg. A, B, C...) and the "vv" is the type identifier. If the product is RoHS compliant, "L" can be found at the end of the part number.

 $USB-6210/6211/6212/6215/6216/6218/6212\ MASS\ TERMINATION/6216\ MASS\ TERMINATION - Label\ can\ be\ found\ on\ the\ bottom\ of\ the\ enclosure.$

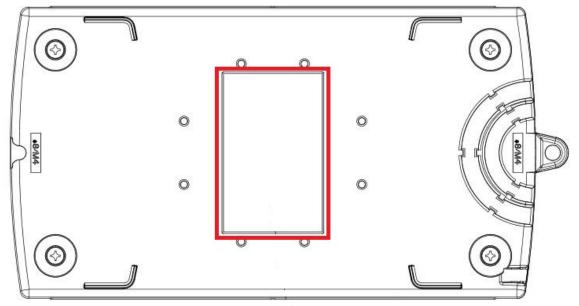


USB-6211 OEM/6218 OEM - Primary Side

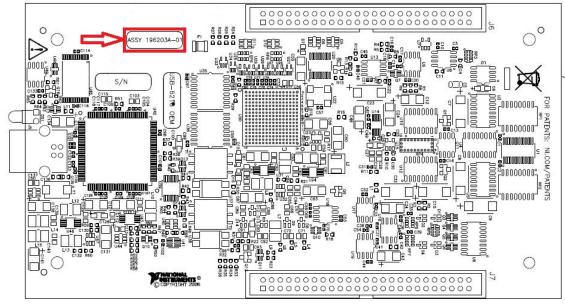

April 2017 376679A-01 Rev 001 Notice: This document is subject to change without notice. For the most recent version, visit ni.com/manuals.



USB-6212 OEM/6216 OEM - Secondary Side

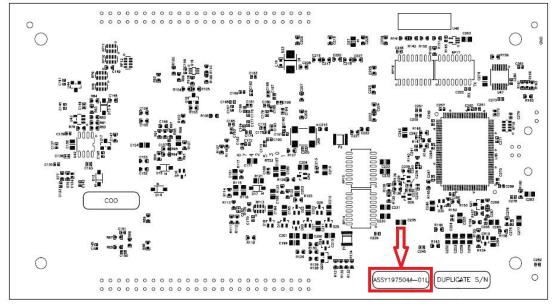

USB-6212 BNC/6216 BNC/6218 BNC - Label can be found on the bottom of the enclosure.



Procedure 2 – Device Configuration EEPROM (Calibration Metadata):

The user-accessible areas of the Device Configuration EEPROM are exposed through a calibration Applications Programming Interface (API) in LabVIEW. To clear the Calibration Metadata area, complete the following steps:

- 1. To clear the calibration password, use the DAQmx Change External Calibration Password.vi to overwrite the current password of the device you wish to clear.
- 2. The user-accessible area of the Device Configuration EEPROM can be cleared using the NI DAQmx API. For instructions on how to clear these areas, go to <u>www.ni.com/info</u> and enter info code *DAQmxLOV*.



Terms and Definitions

Cycle Power:

The process of completely removing power from the device and its components and allowing for adequate discharge. This process includes a complete shutdown of the PC and/or chassis containing the device; a reboot is not sufficient for the completion of this process.

Volatile Memory:

Requires power to maintain the stored information. When power is removed from this memory, its contents are lost. This type of memory typically contains application specific data such as capture waveforms.

Non-Volatile Memory:

Power is not required to maintain the stored information. Device retains its contents when power is removed. This type of memory typically contains information necessary to boot, configure, or calibrate the product or may include device power up states.

User Accessible:

The component is read and/or write addressable such that a user can store arbitrary information to the component from the host using a publicly distributed NI tool, such as a Driver API, the System Configuration API, or MAX.

System Accessible:

The component is read and/or write addressable from the host without the need to physically alter the product.

Clearing:

Per *NIST Special Publication 800-88 Revision 1*, "clearing" is a logical technique to sanitize data in all User Accessible storage locations for protection against simple non-invasive data recovery techniques using the same interface available to the user; typically applied through the standard read and write commands to the storage device.

Sanitization:

Per *NIST Special Publication 800-88 Revision 1*, "sanitization" is a process to render access to "Target Data" on the media infeasible for a given level of effort. In this document, clearing is the degree of sanitization described.